
SAMPLE INFORMATION

Sample Name:	AV320-SO-Blank	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 av407 blanks
Vial:	70	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-23 15:31:27 CET		
Date Processed:	2025-01-24 07:48:30 CET		

Auto-Scaled Chromatogram

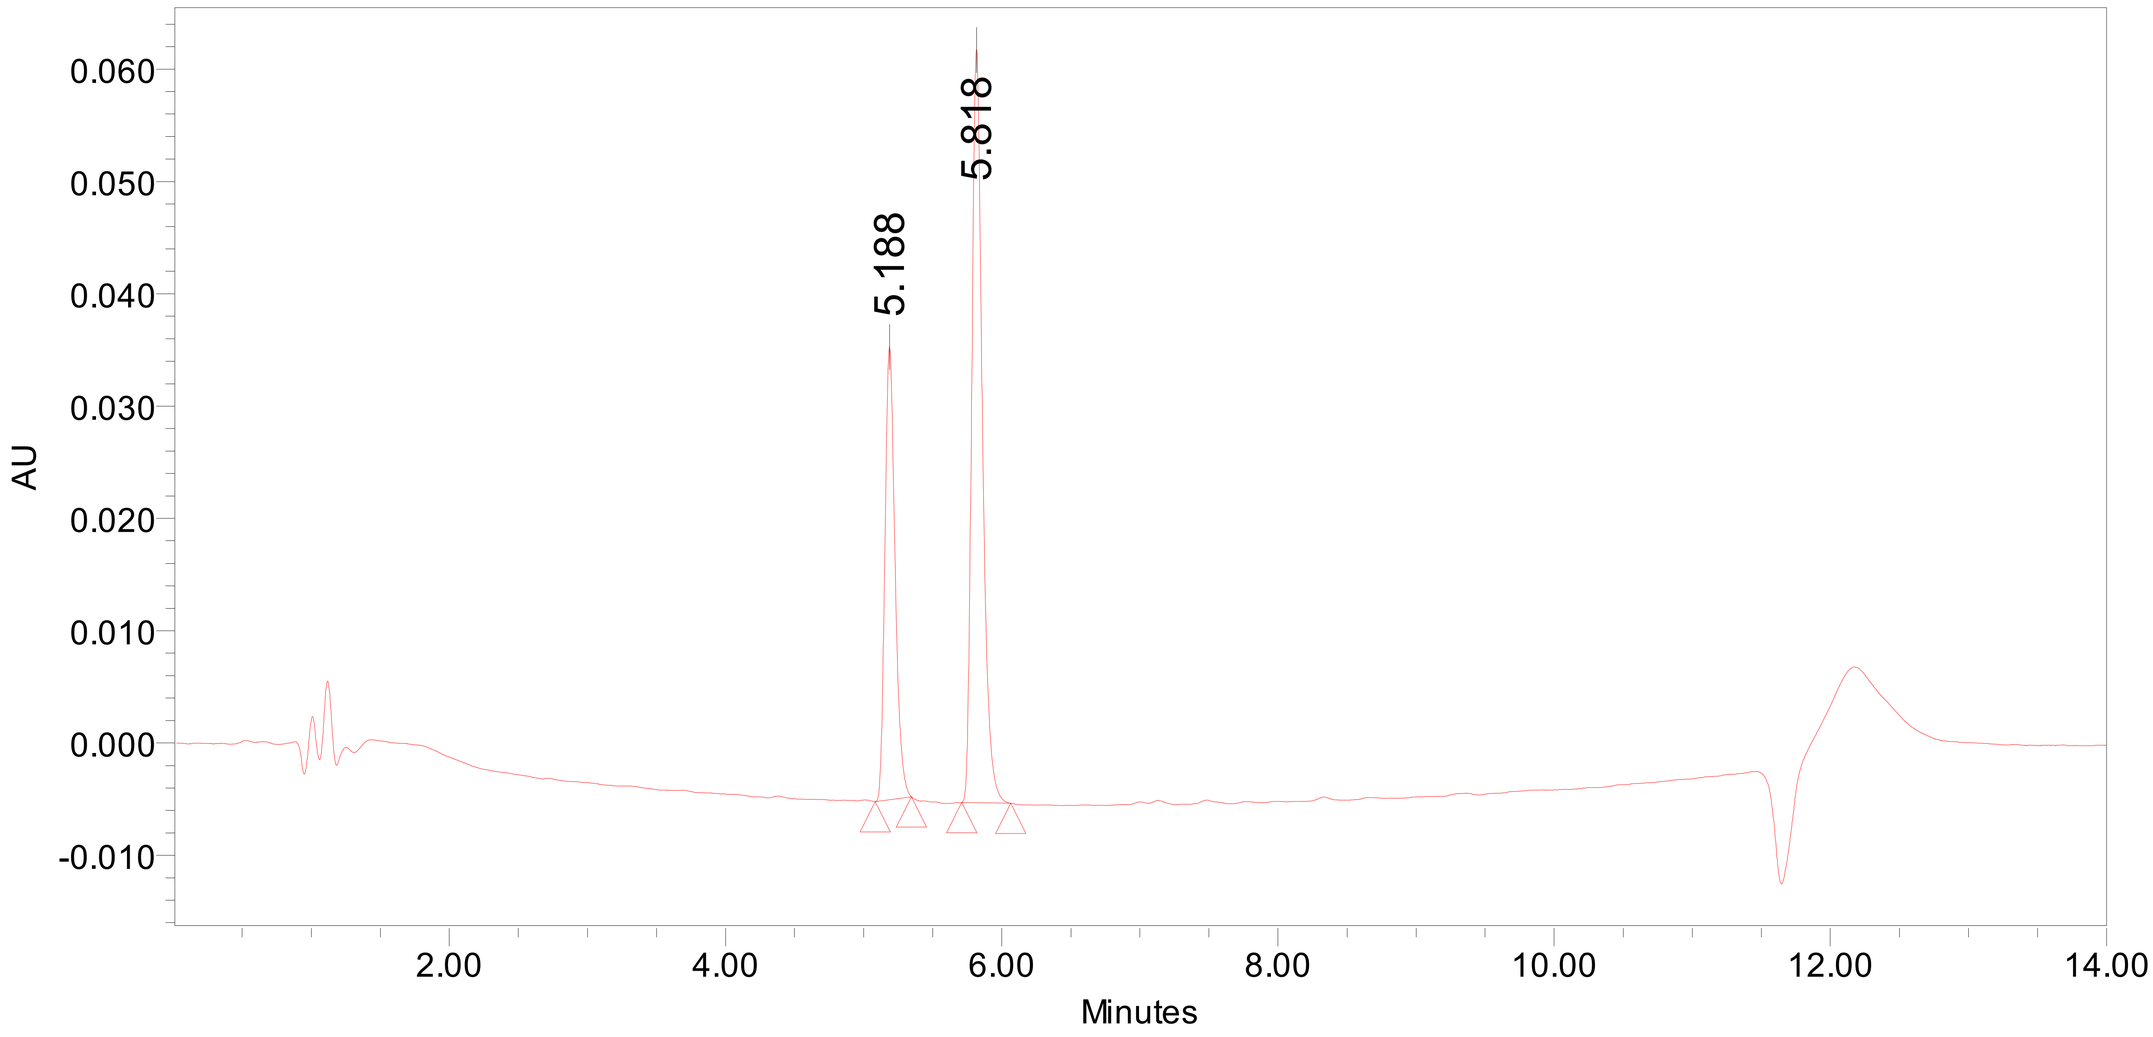

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.188	204943	40304		
2		5.818	360812	67069		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.188					
2		5.818					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-15 min correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-27 18:28:02 CET		
Date Processed:	2025-02-28 09:33:11 CET		

Auto-Scaled Chromatogram

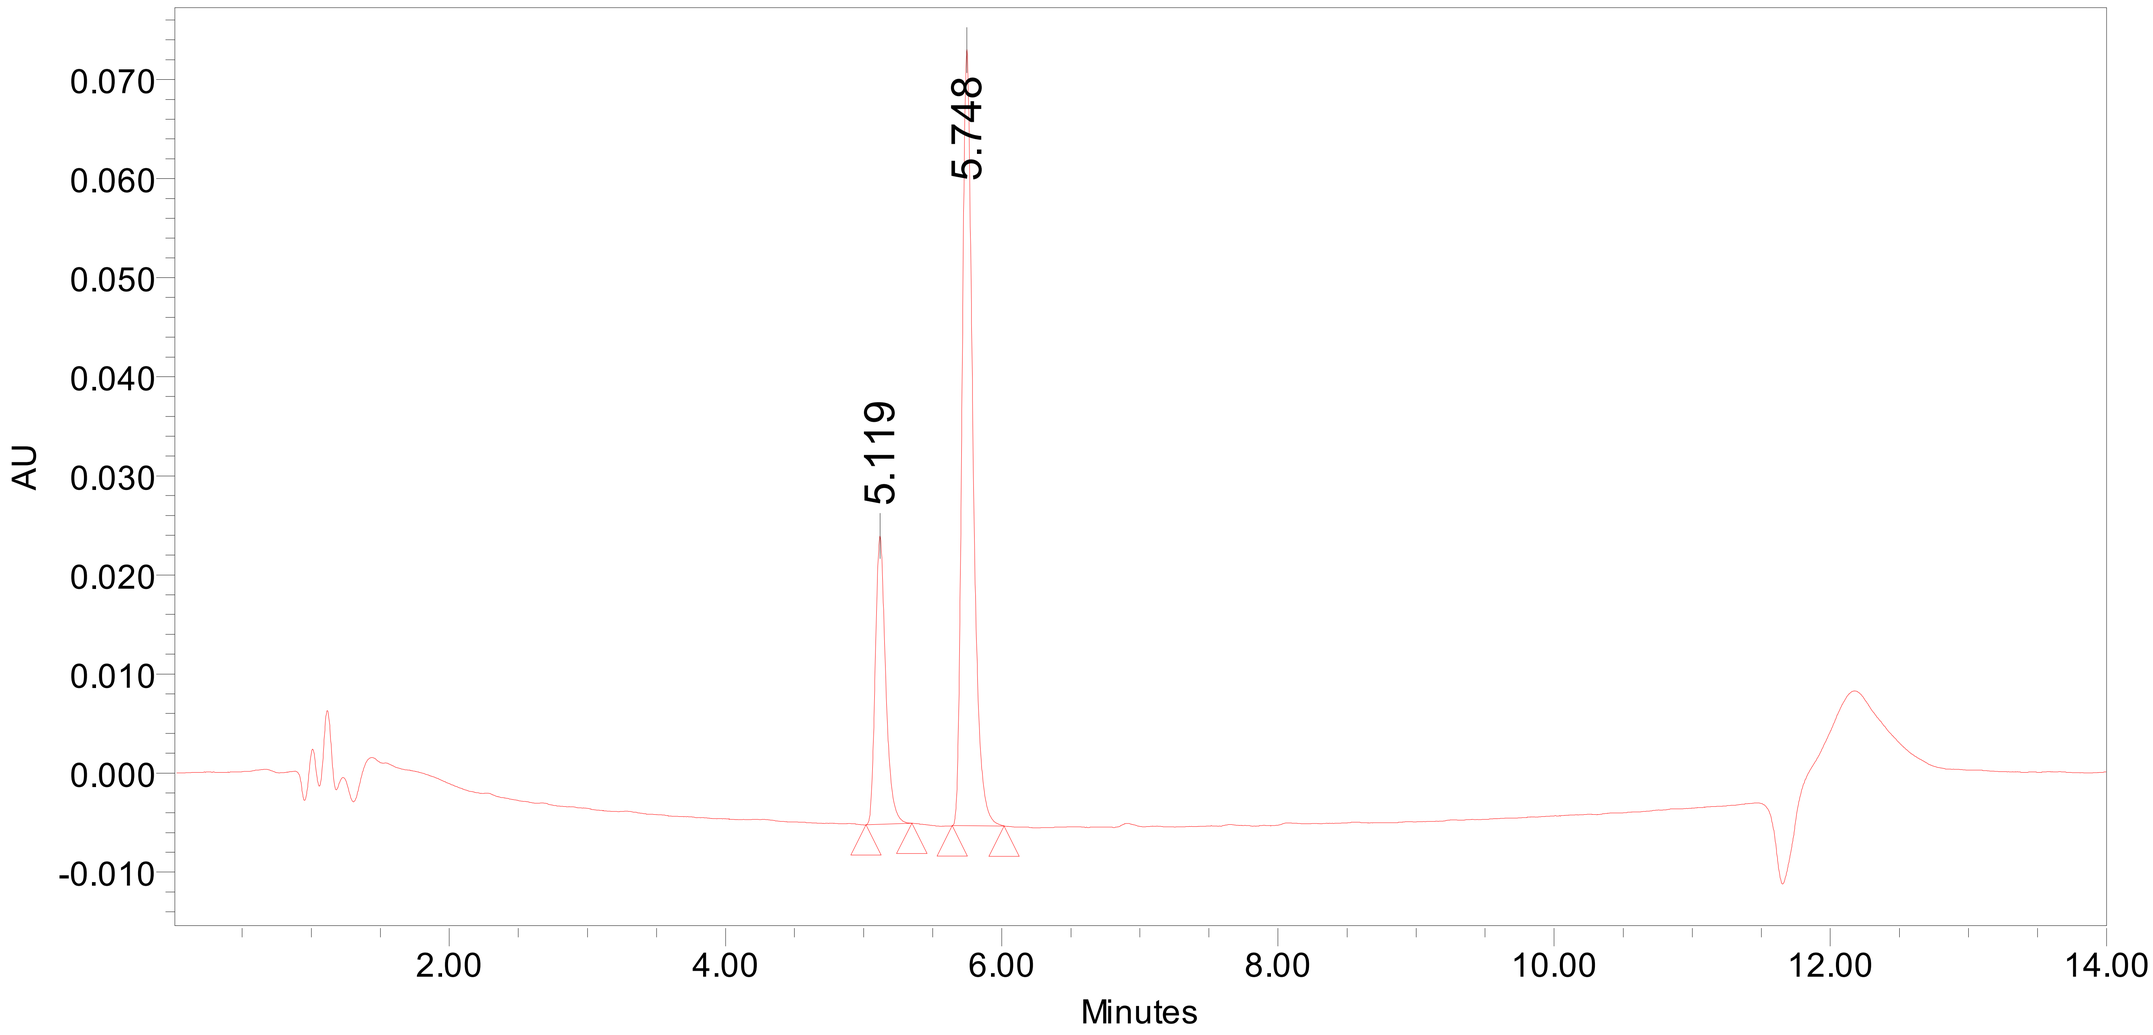

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.119	152772	29124		
2		5.748	429591	78366		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.119					
2		5.748					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-1 h-correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-27 19:31:29 CET		
Date Processed:	2025-02-28 09:33:29 CET		

Auto-Scaled Chromatogram

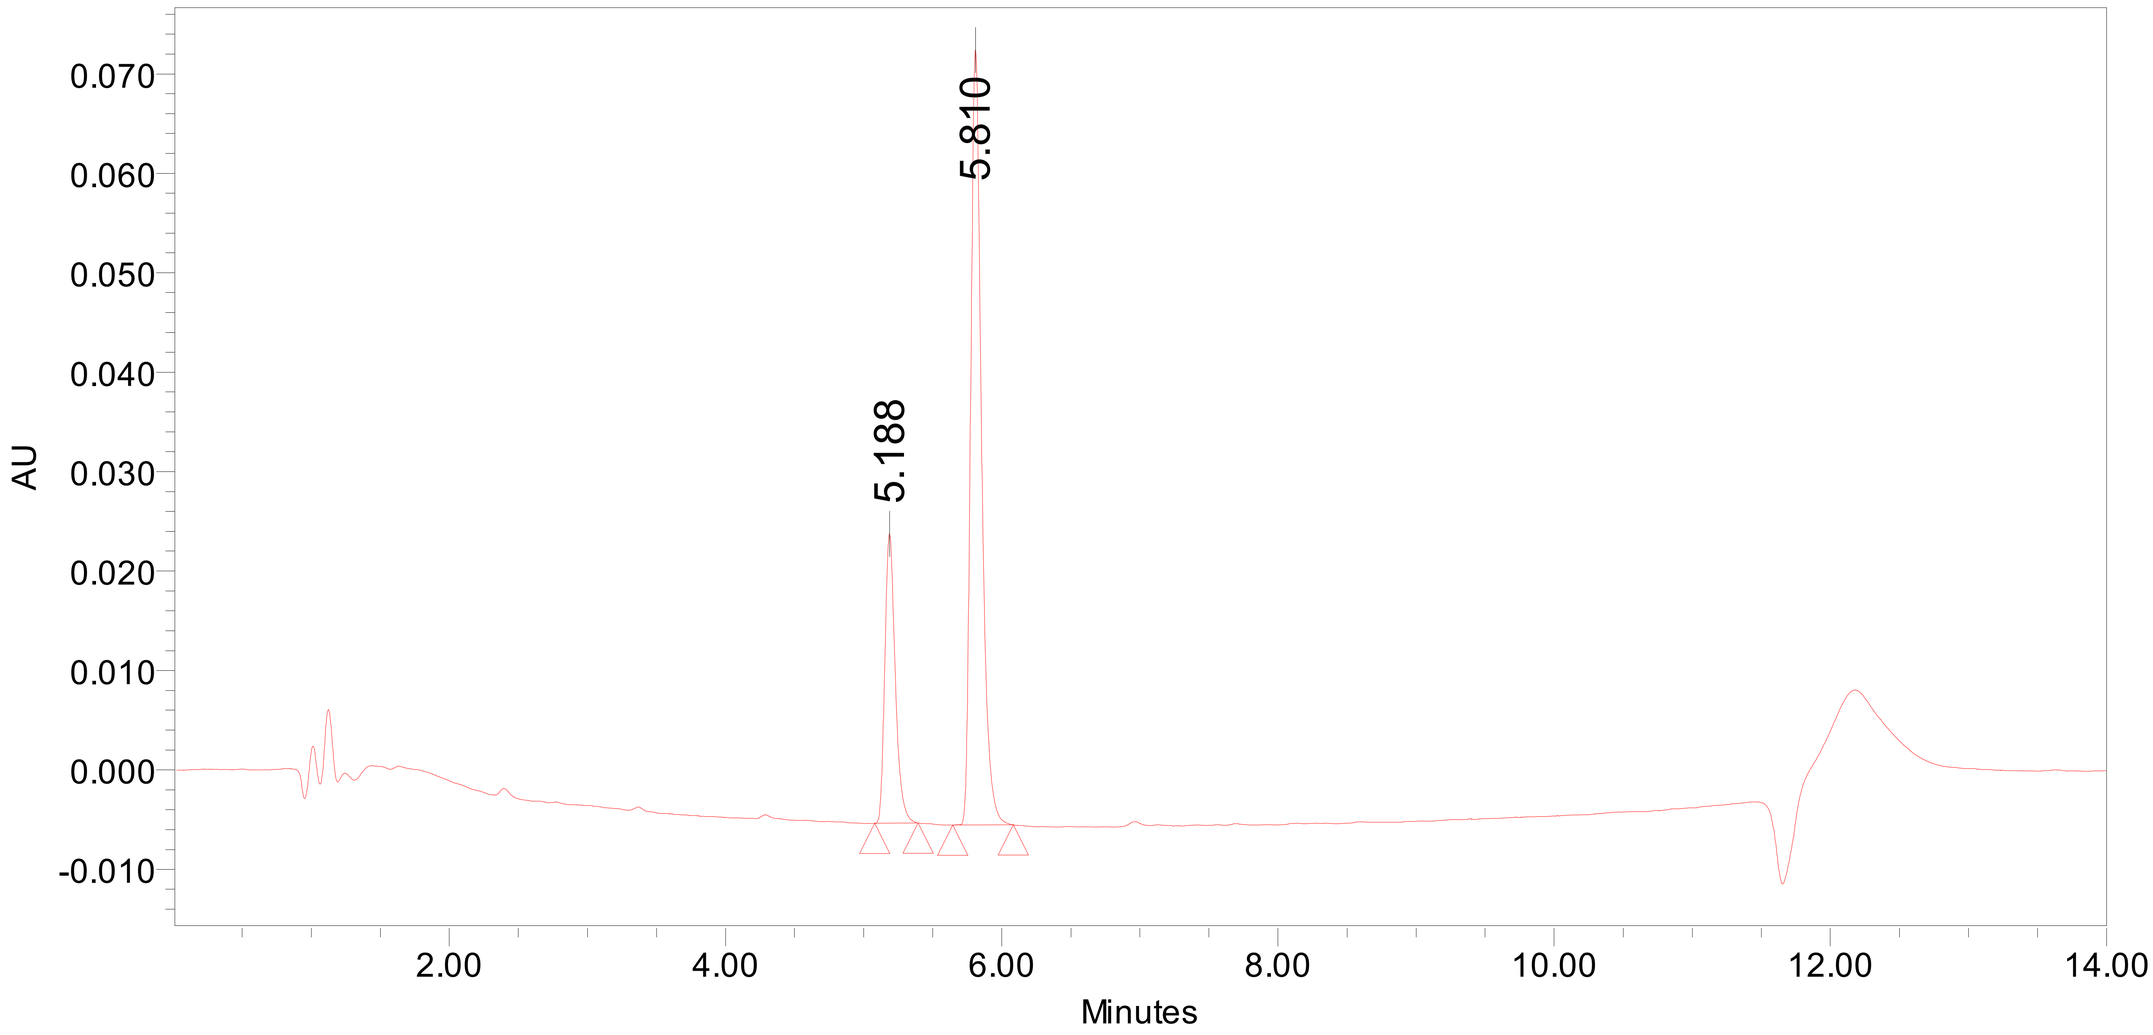

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.188	151986	29125		
2		5.810	426278	77992		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.188					
2		5.810					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-2 h-correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-27 20:34:51 CET		
Date Processed:	2025-02-28 09:33:45 CET		

Auto-Scaled Chromatogram

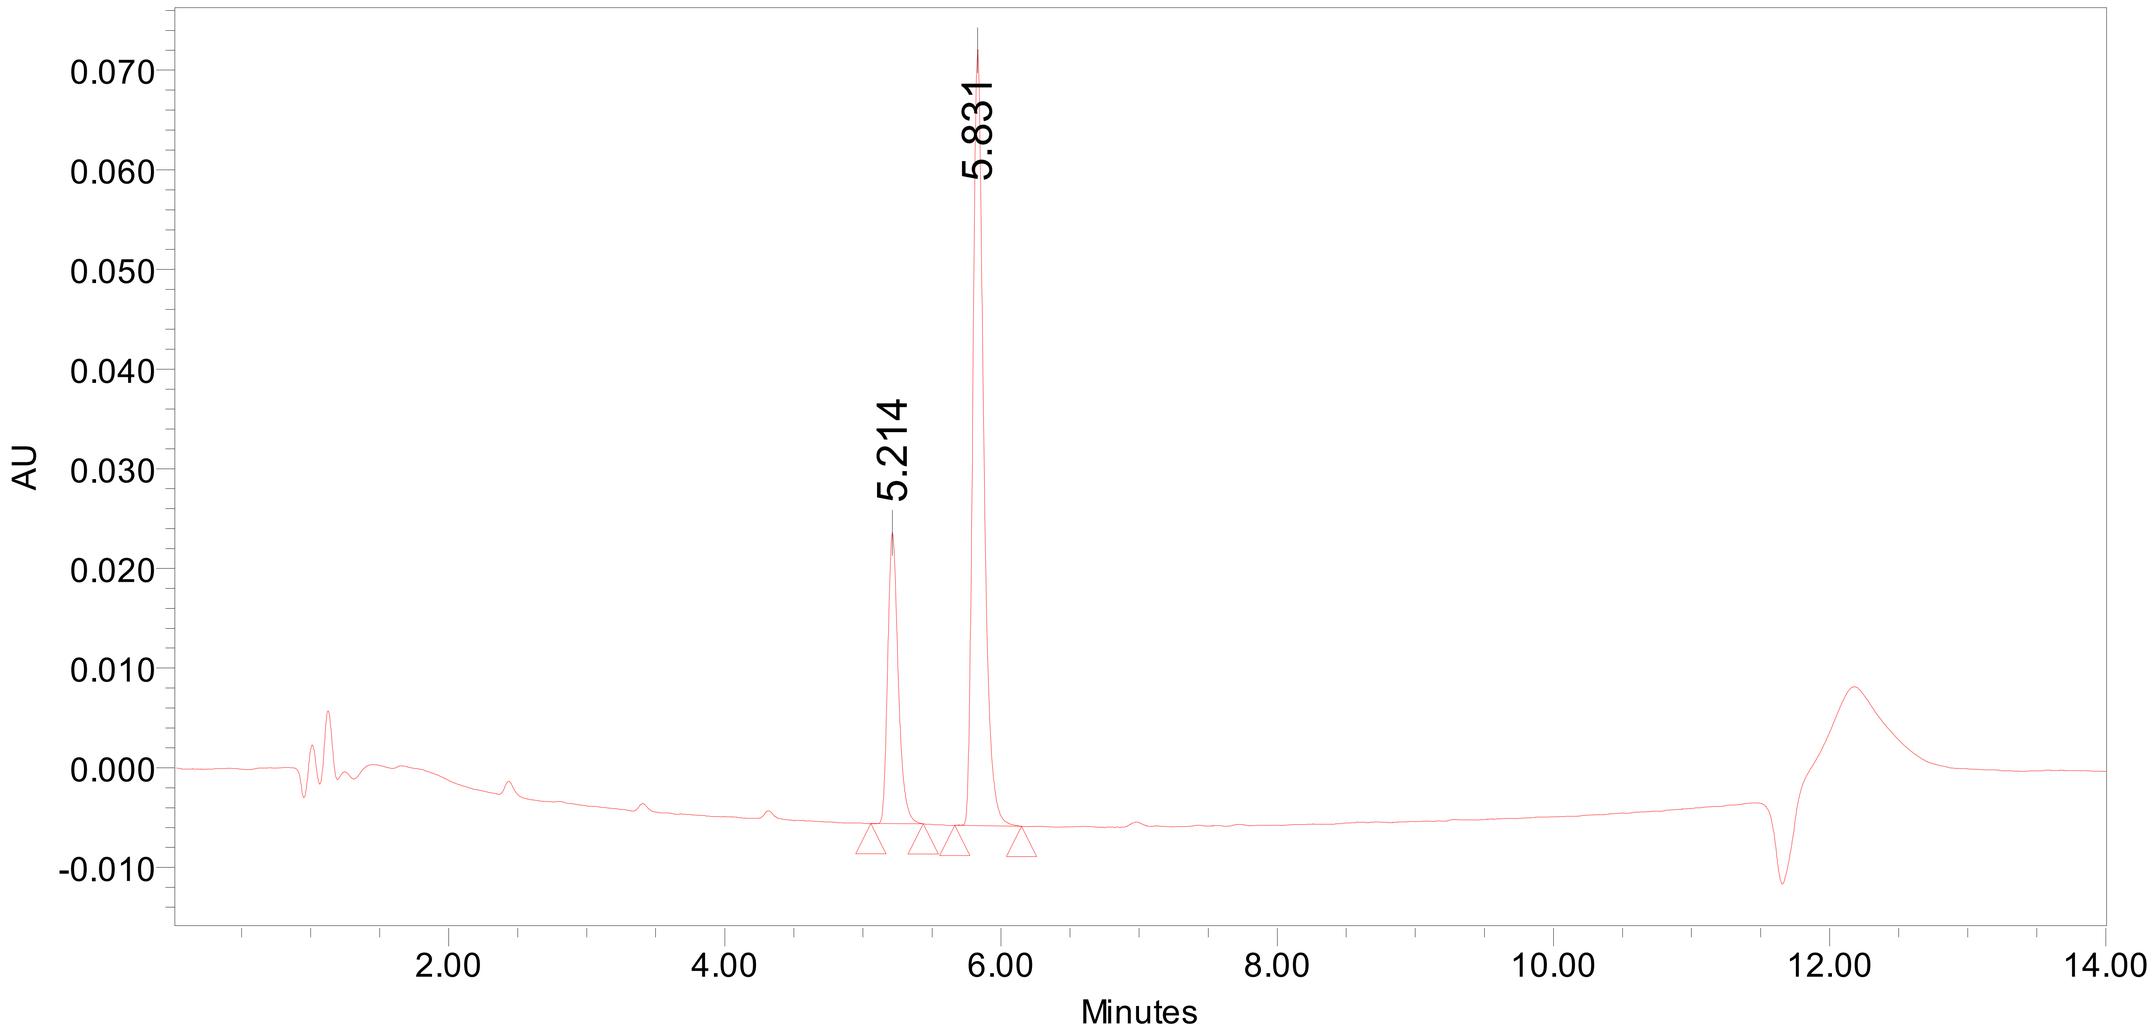

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.214	153781	29233		
2		5.831	427612	77912		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.214					
2		5.831					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-3 h-correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-27 21:38:16 CET		
Date Processed:	2025-02-28 09:34:00 CET		

Auto-Scaled Chromatogram

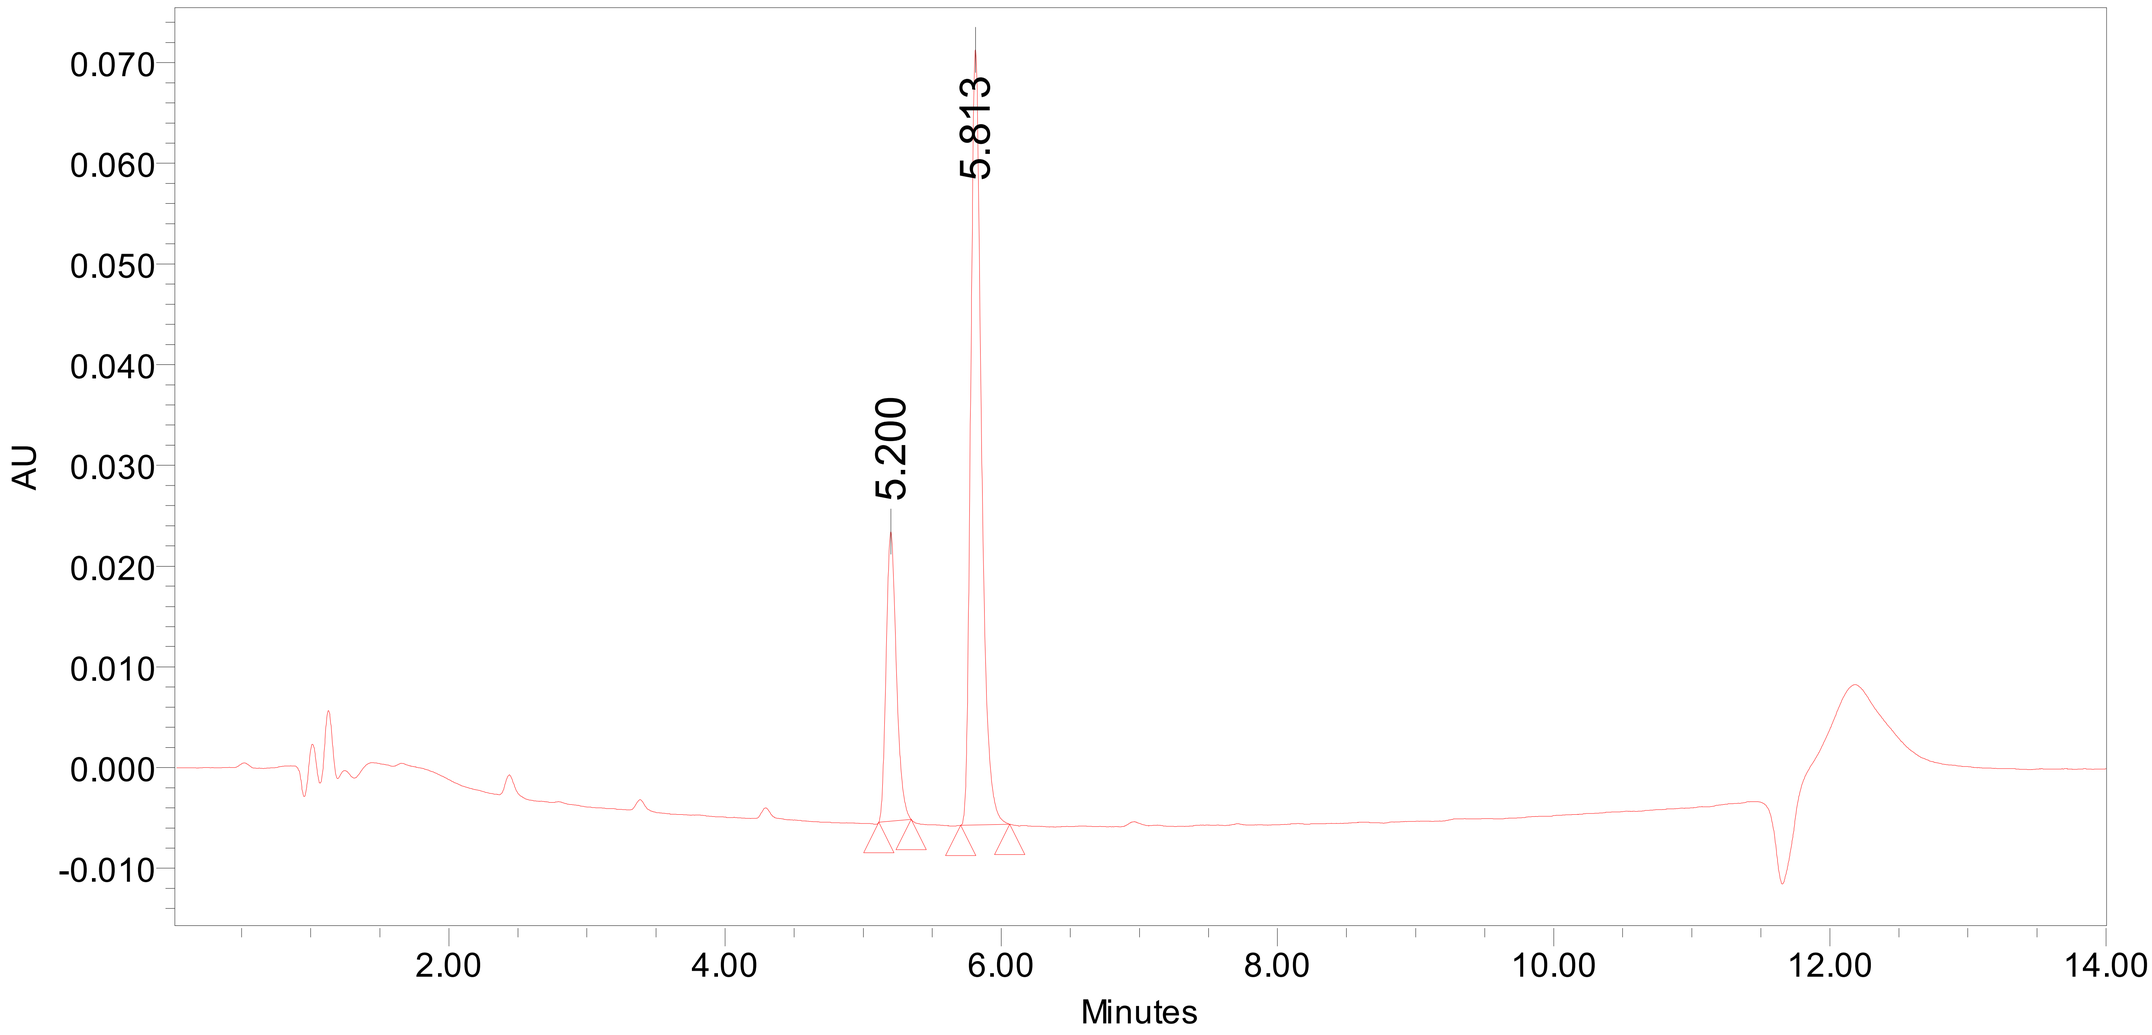

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.200	147170	28763		
2		5.813	419564	77009		

PDA Result Table


	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.200					
2		5.813					

Untitled

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-4 h-correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-27 22:41:40 CET		
Date Processed:	2025-02-28 09:34:16 CET		

Auto-Scaled Chromatogram

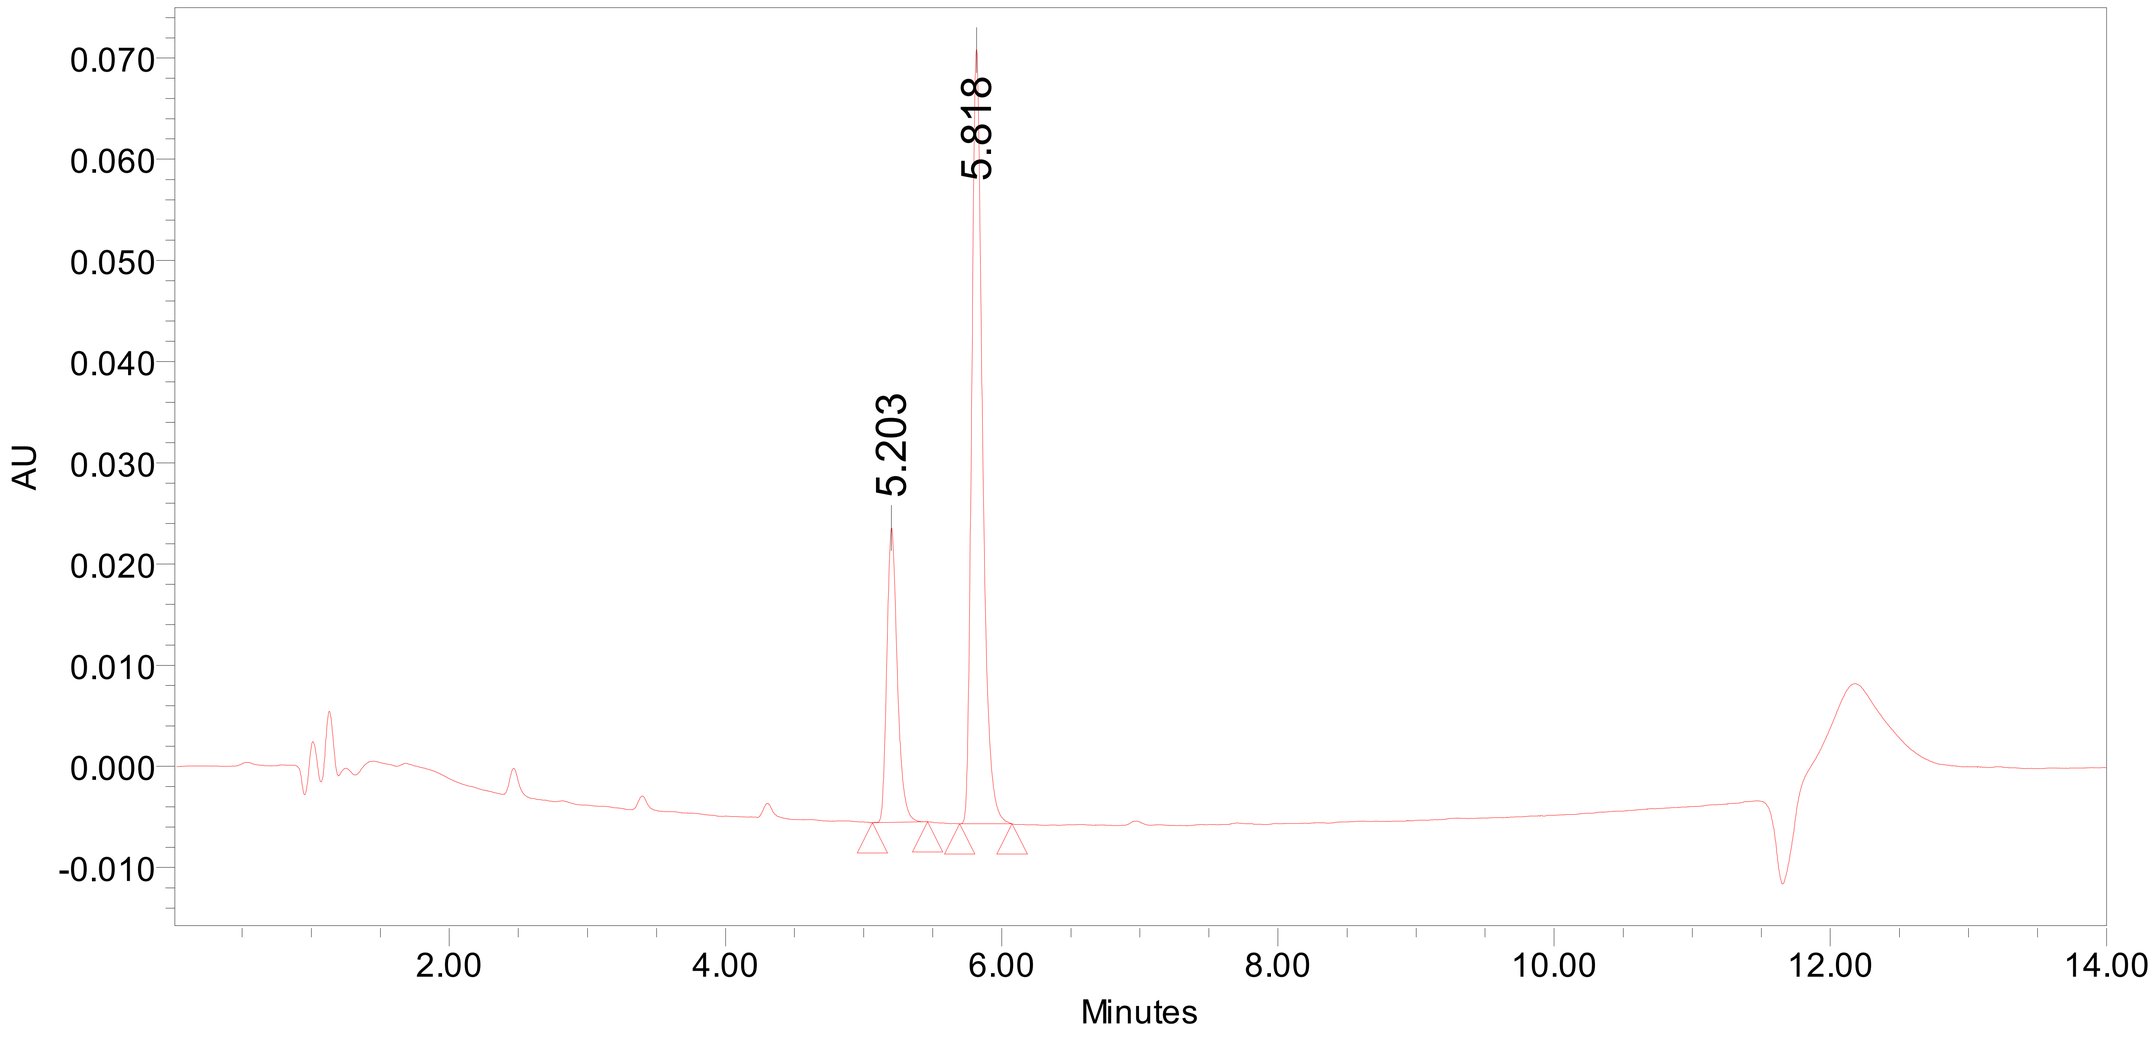

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.203	152061	29091		
2		5.818	418223	76528		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.203					
2		5.818					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-6 h-correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-28 00:30:02 CET		
Date Processed:	2025-02-28 09:34:31 CET		

Auto-Scaled Chromatogram

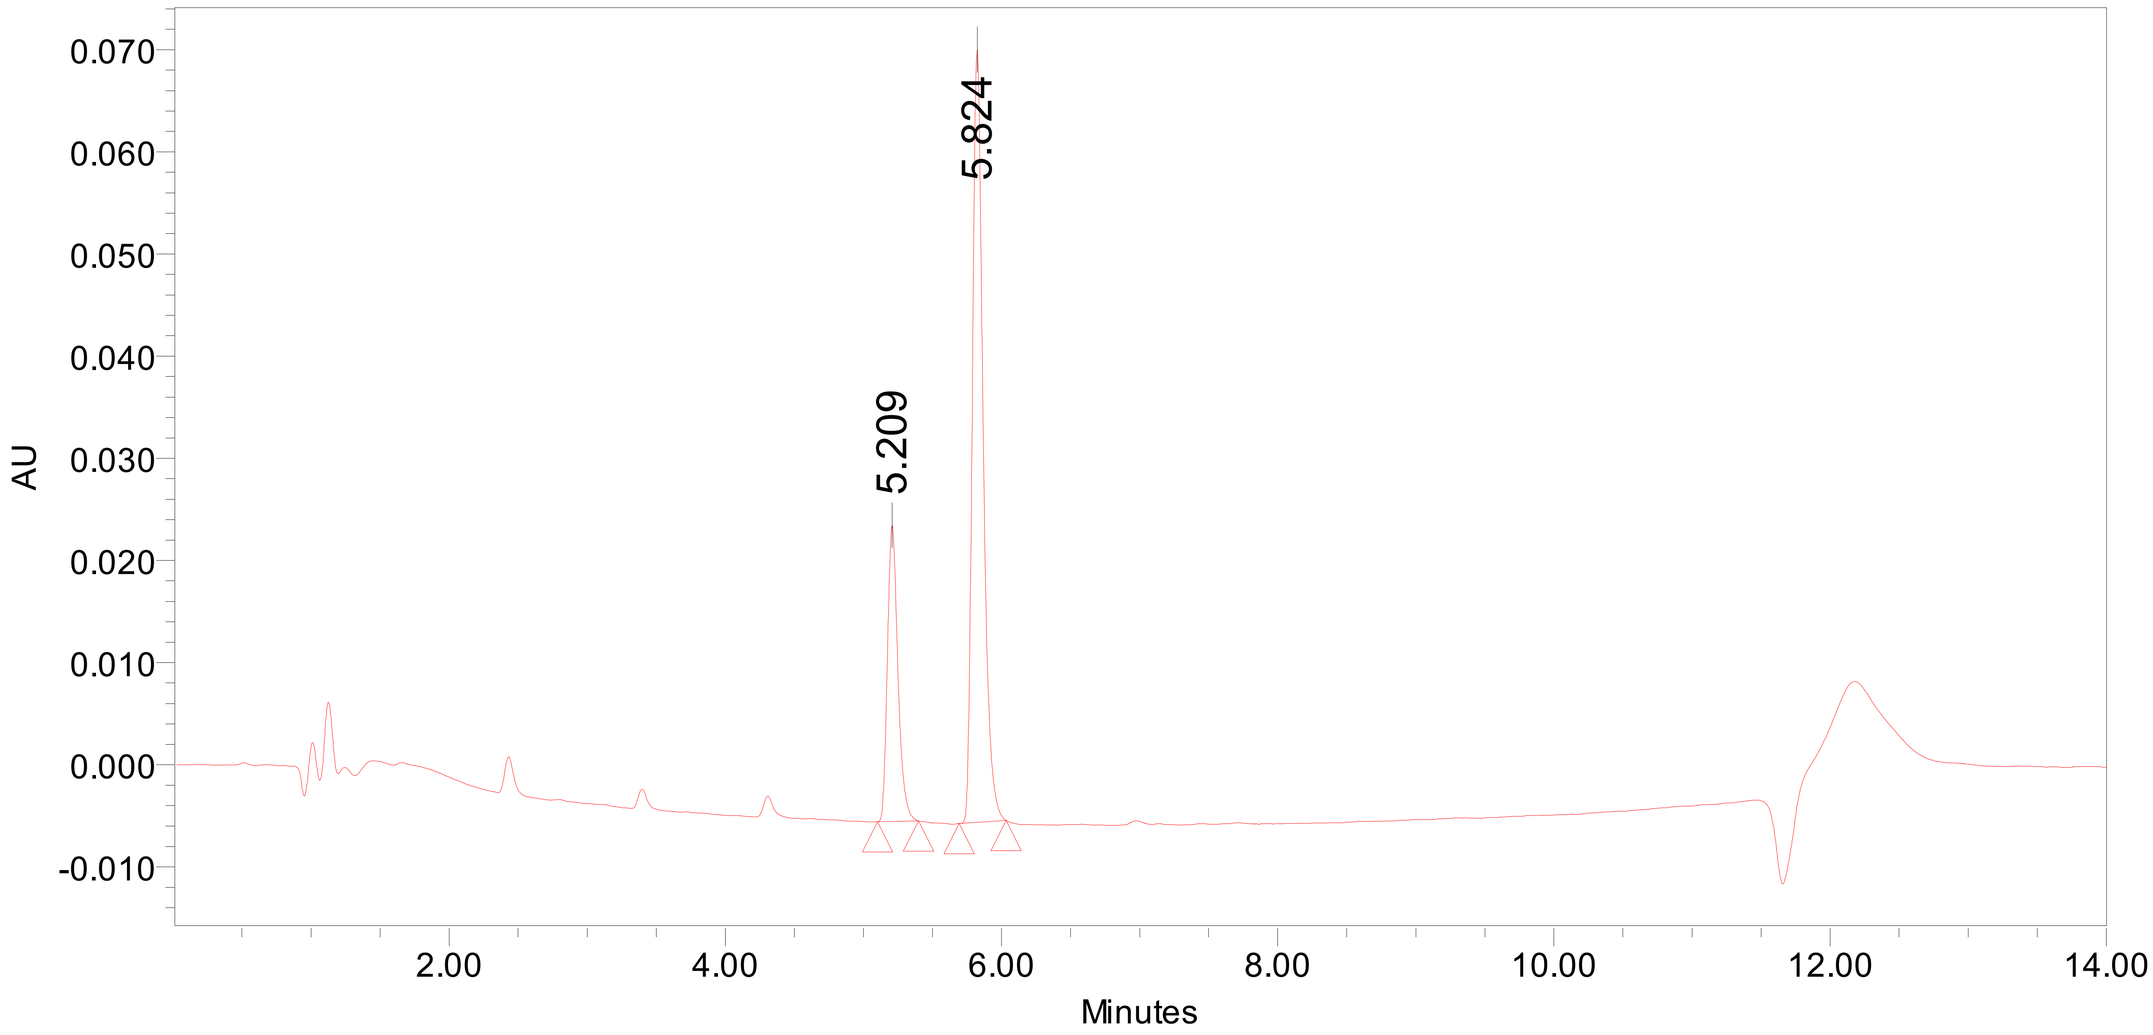

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.209	151622	29004		
2		5.824	411442	75674		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.209					
2		5.824					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-8 h correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-28 02:18:26 CET		
Date Processed:	2025-02-28 09:34:45 CET		

Auto-Scaled Chromatogram

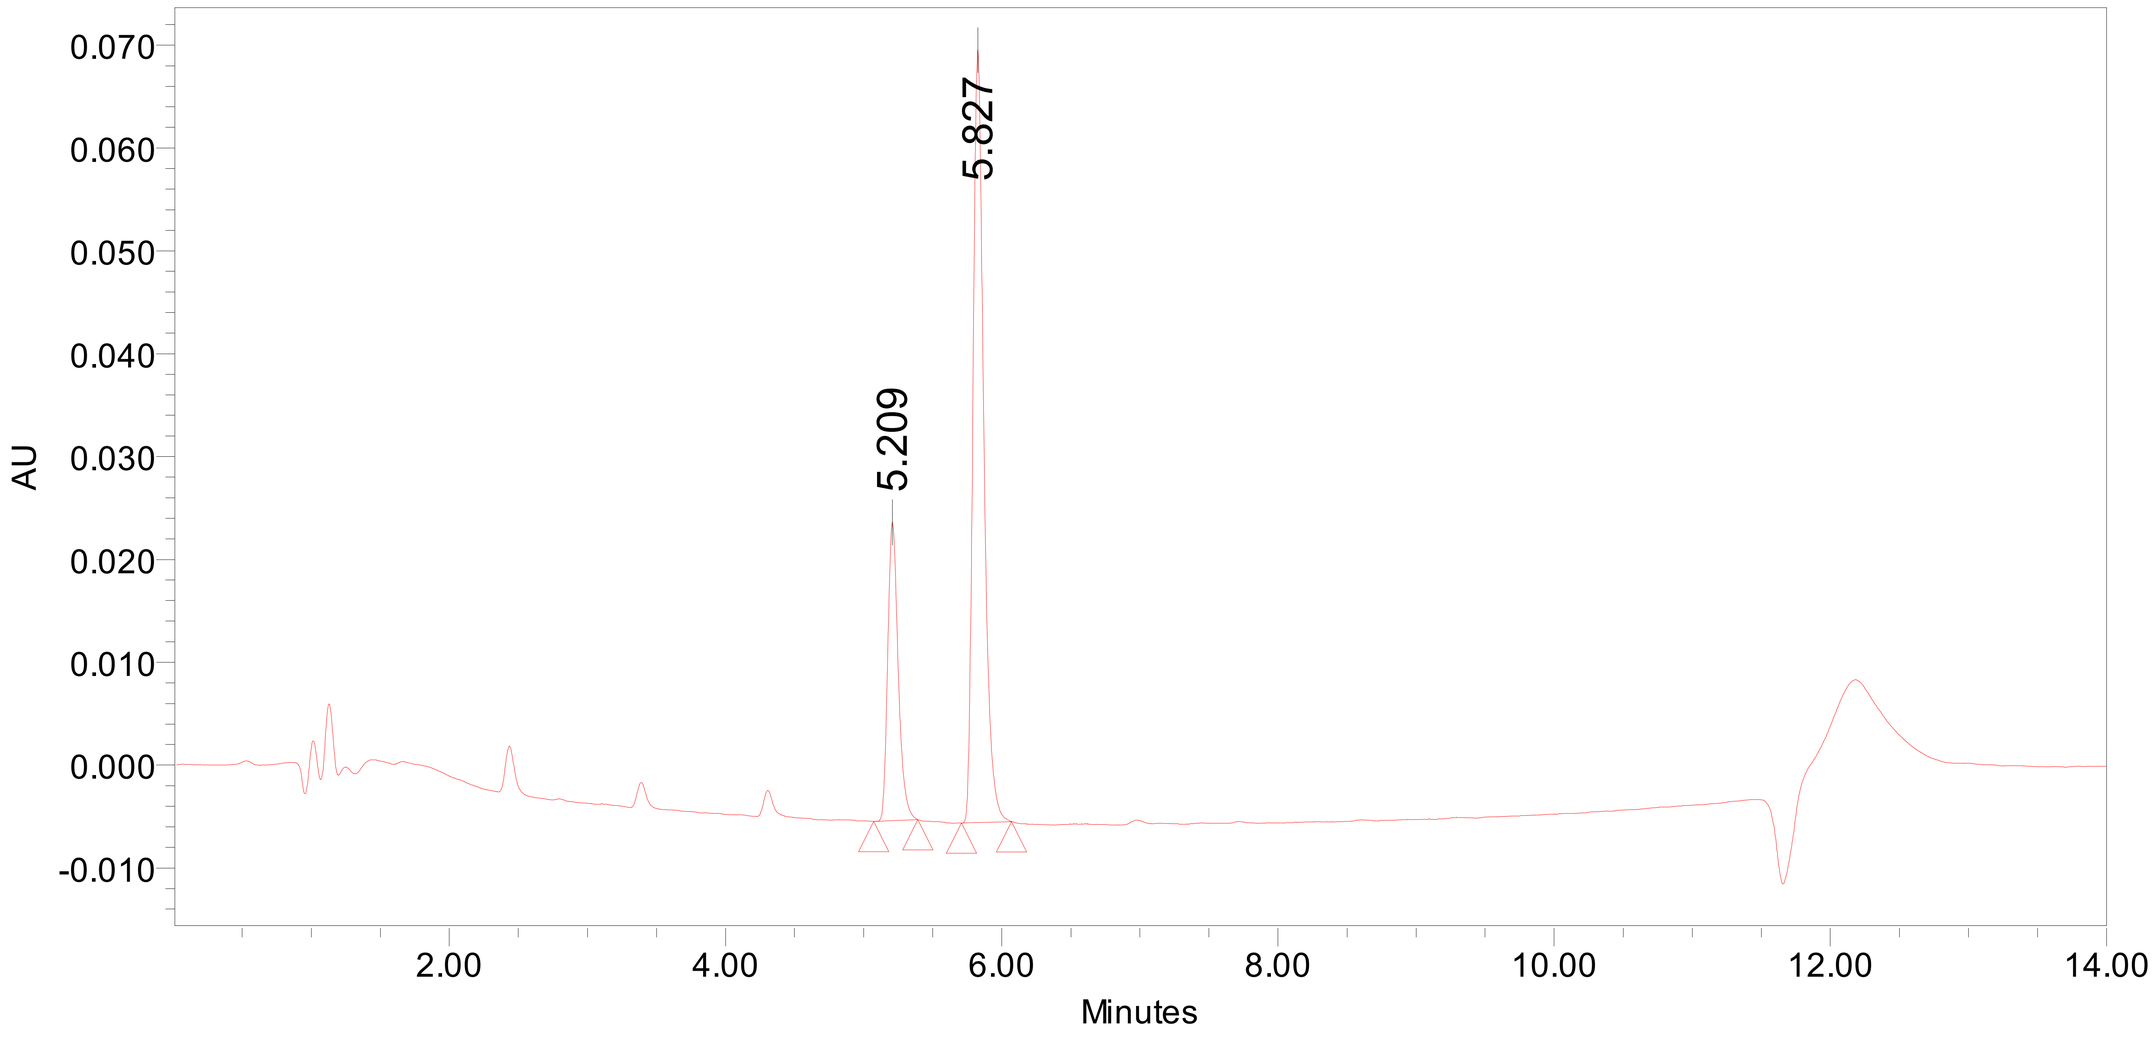

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.209	151701	29045		
2		5.827	410497	75163		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.209					
2		5.827					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-10 h correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-28 04:06:46 CET		
Date Processed:	2025-02-28 09:35:16 CET		

Auto-Scaled Chromatogram

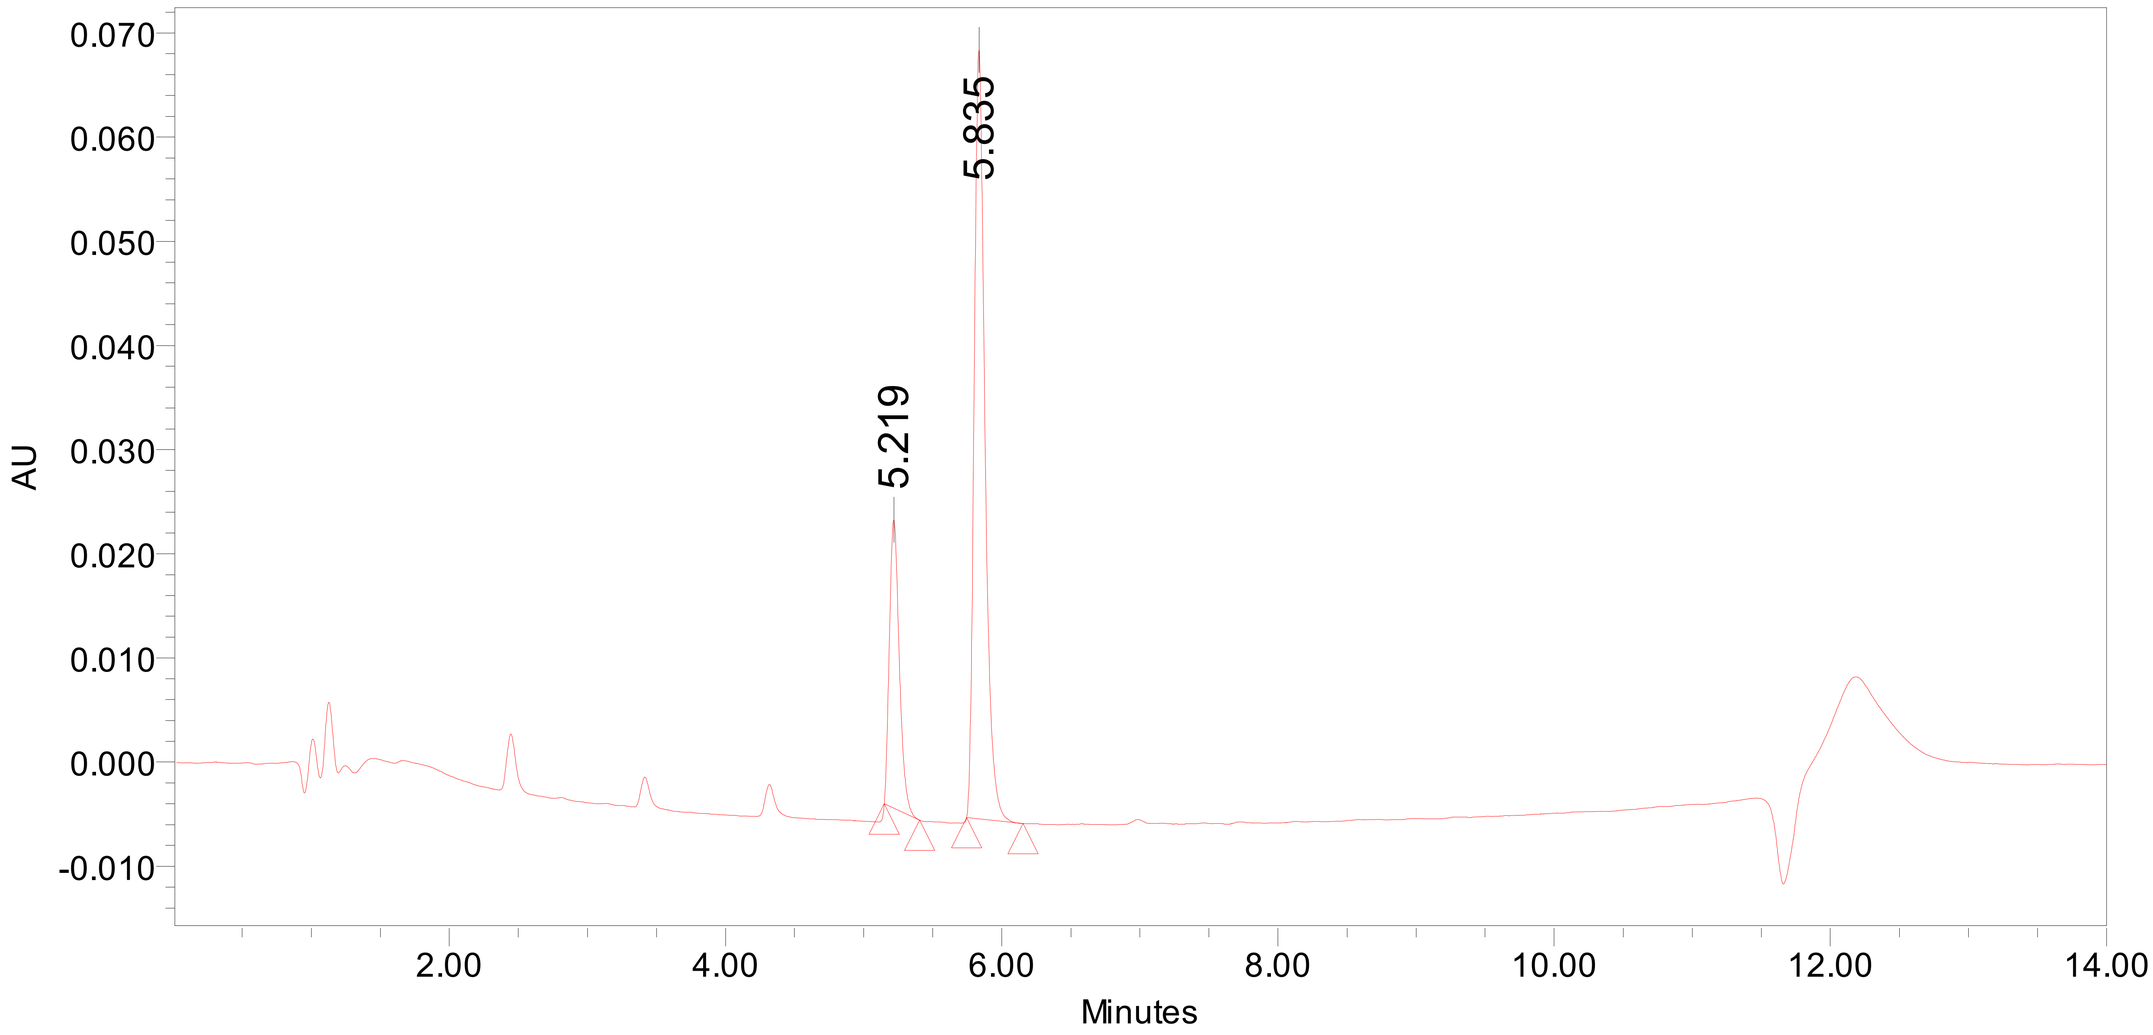

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.219	137239	27695		
2		5.835	401384	73853		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.219					
2		5.835					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-12 h correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-28 05:55:10 CET		
Date Processed:	2025-02-28 09:35:32 CET		

Auto-Scaled Chromatogram

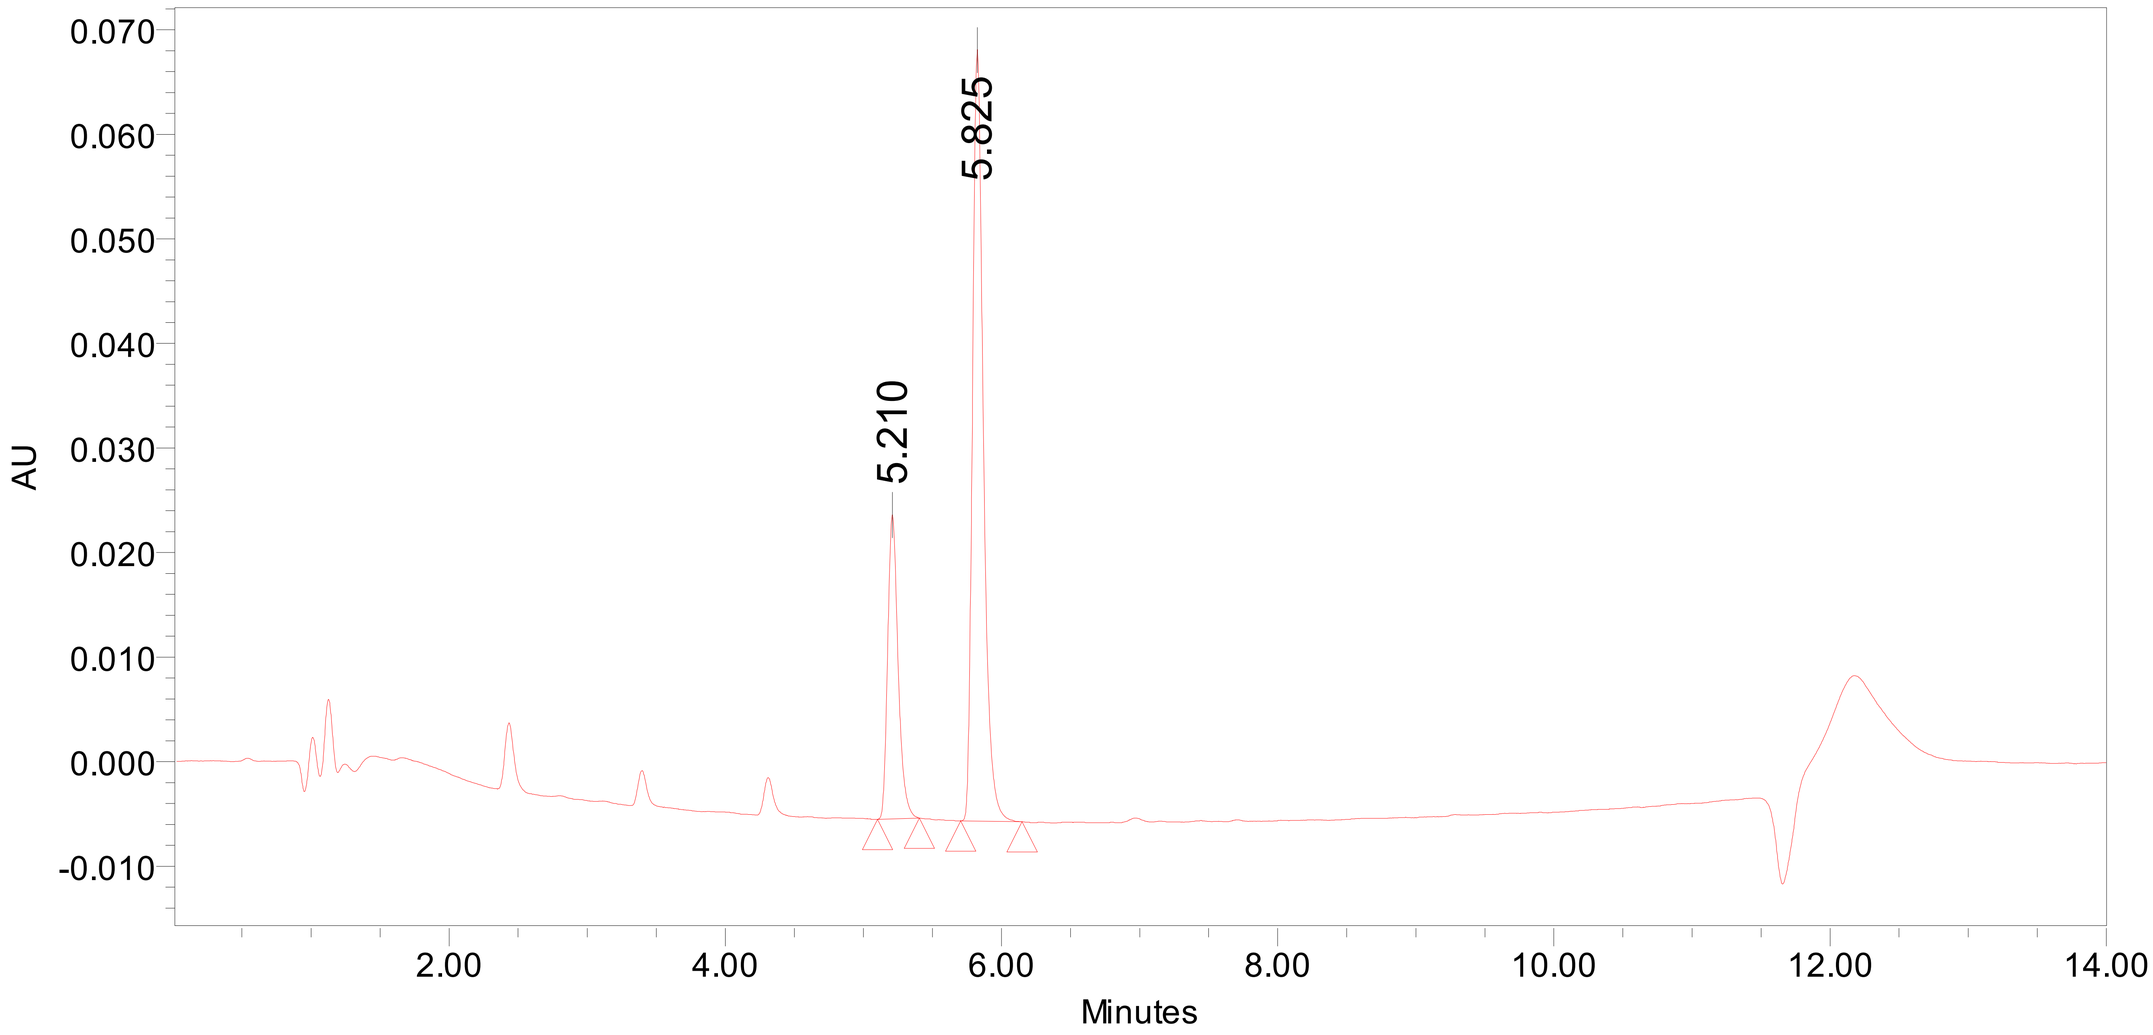

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.210	151857	29076		
2		5.825	404632	73789		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.210					
2		5.825					

SAMPLE INFORMATION

Sample Name:	AV320-SO-NAC-16 h correct	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320 SONAC correct
Vial:	2	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-28 08:30:25 CET		
Date Processed:	2025-02-28 09:35:46 CET		

Auto-Scaled Chromatogram

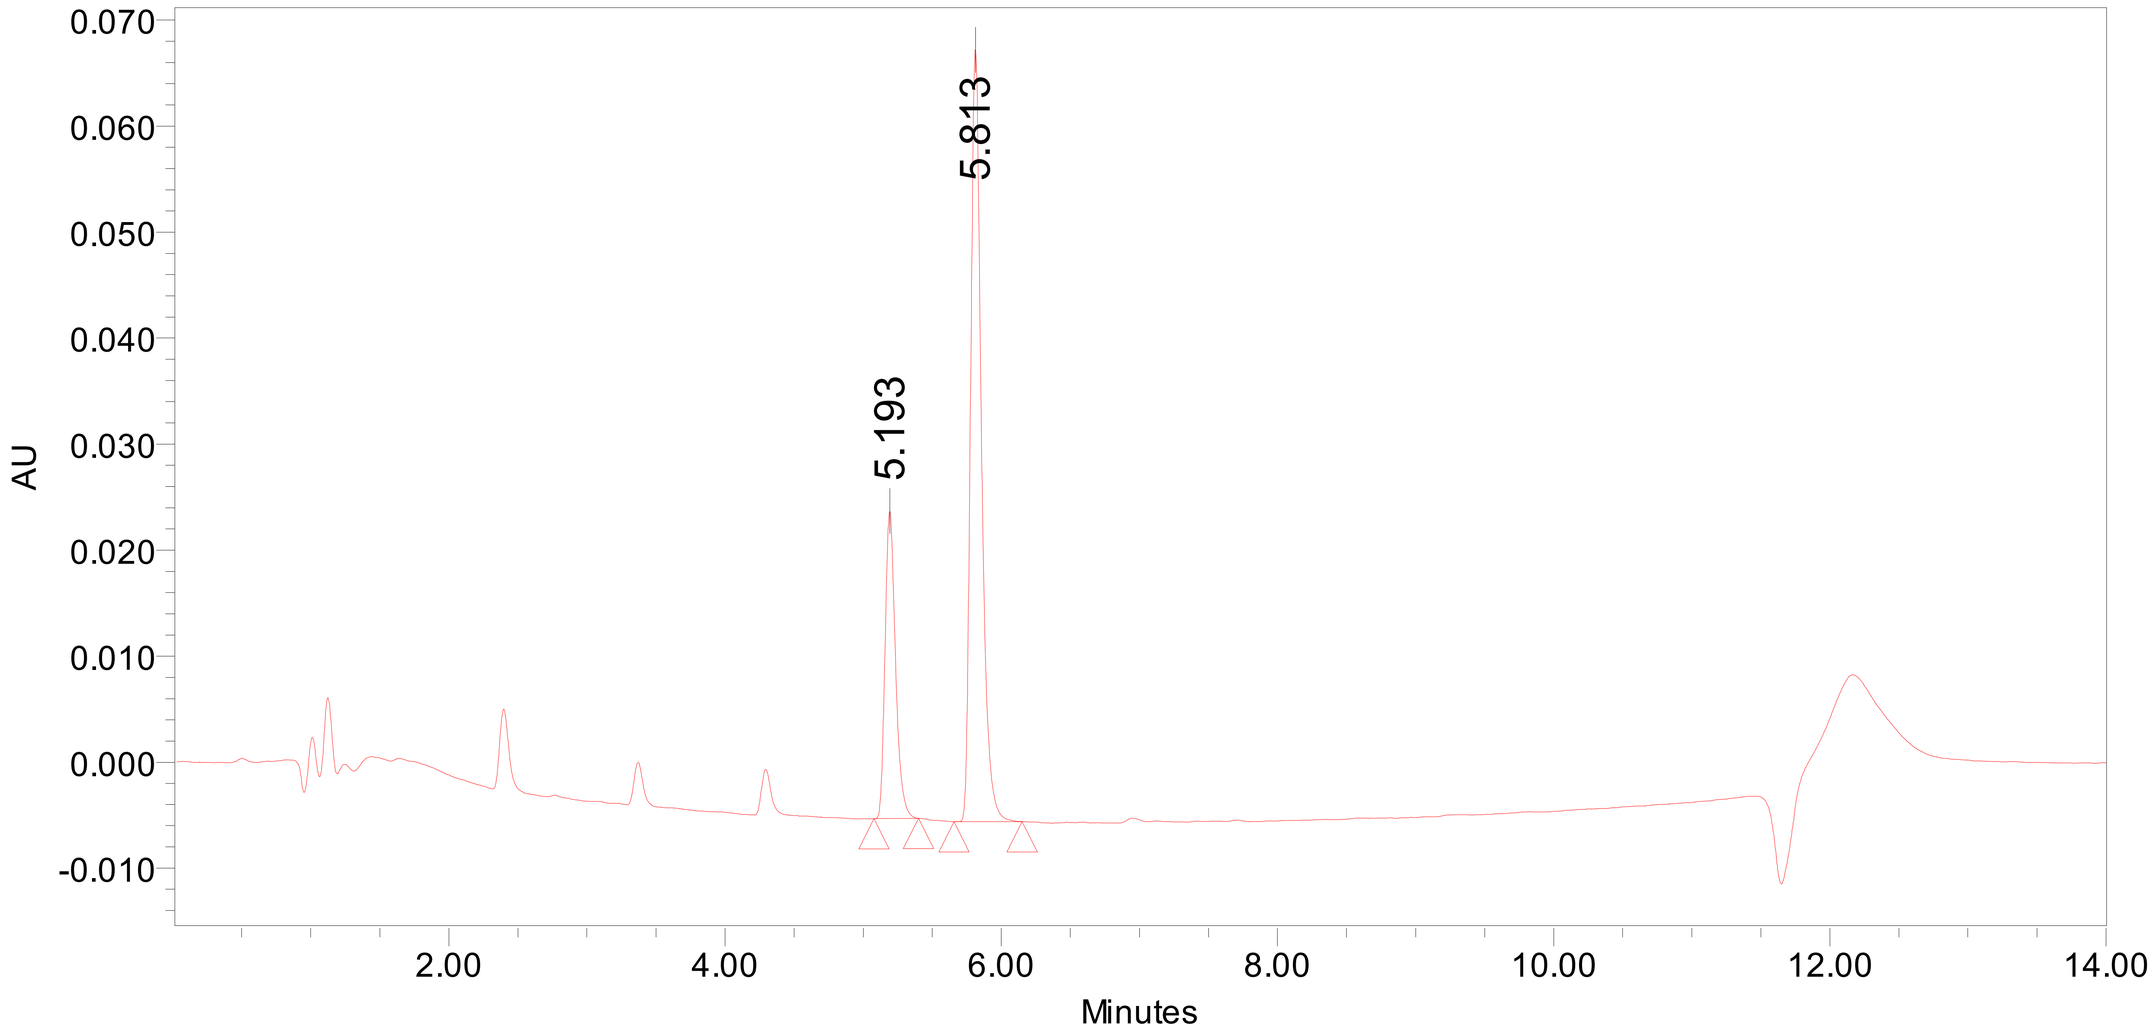

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.193	151744	29032		
2		5.813	398540	72837		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.193					
2		5.813					