
SAMPLE INFORMATION

Sample Name:	HN170-0	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	STABILITY 0
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-07 20:48:29 CET		
Date Processed:	2025-01-17 14:26:41 CET		

Auto-Scaled Chromatogram

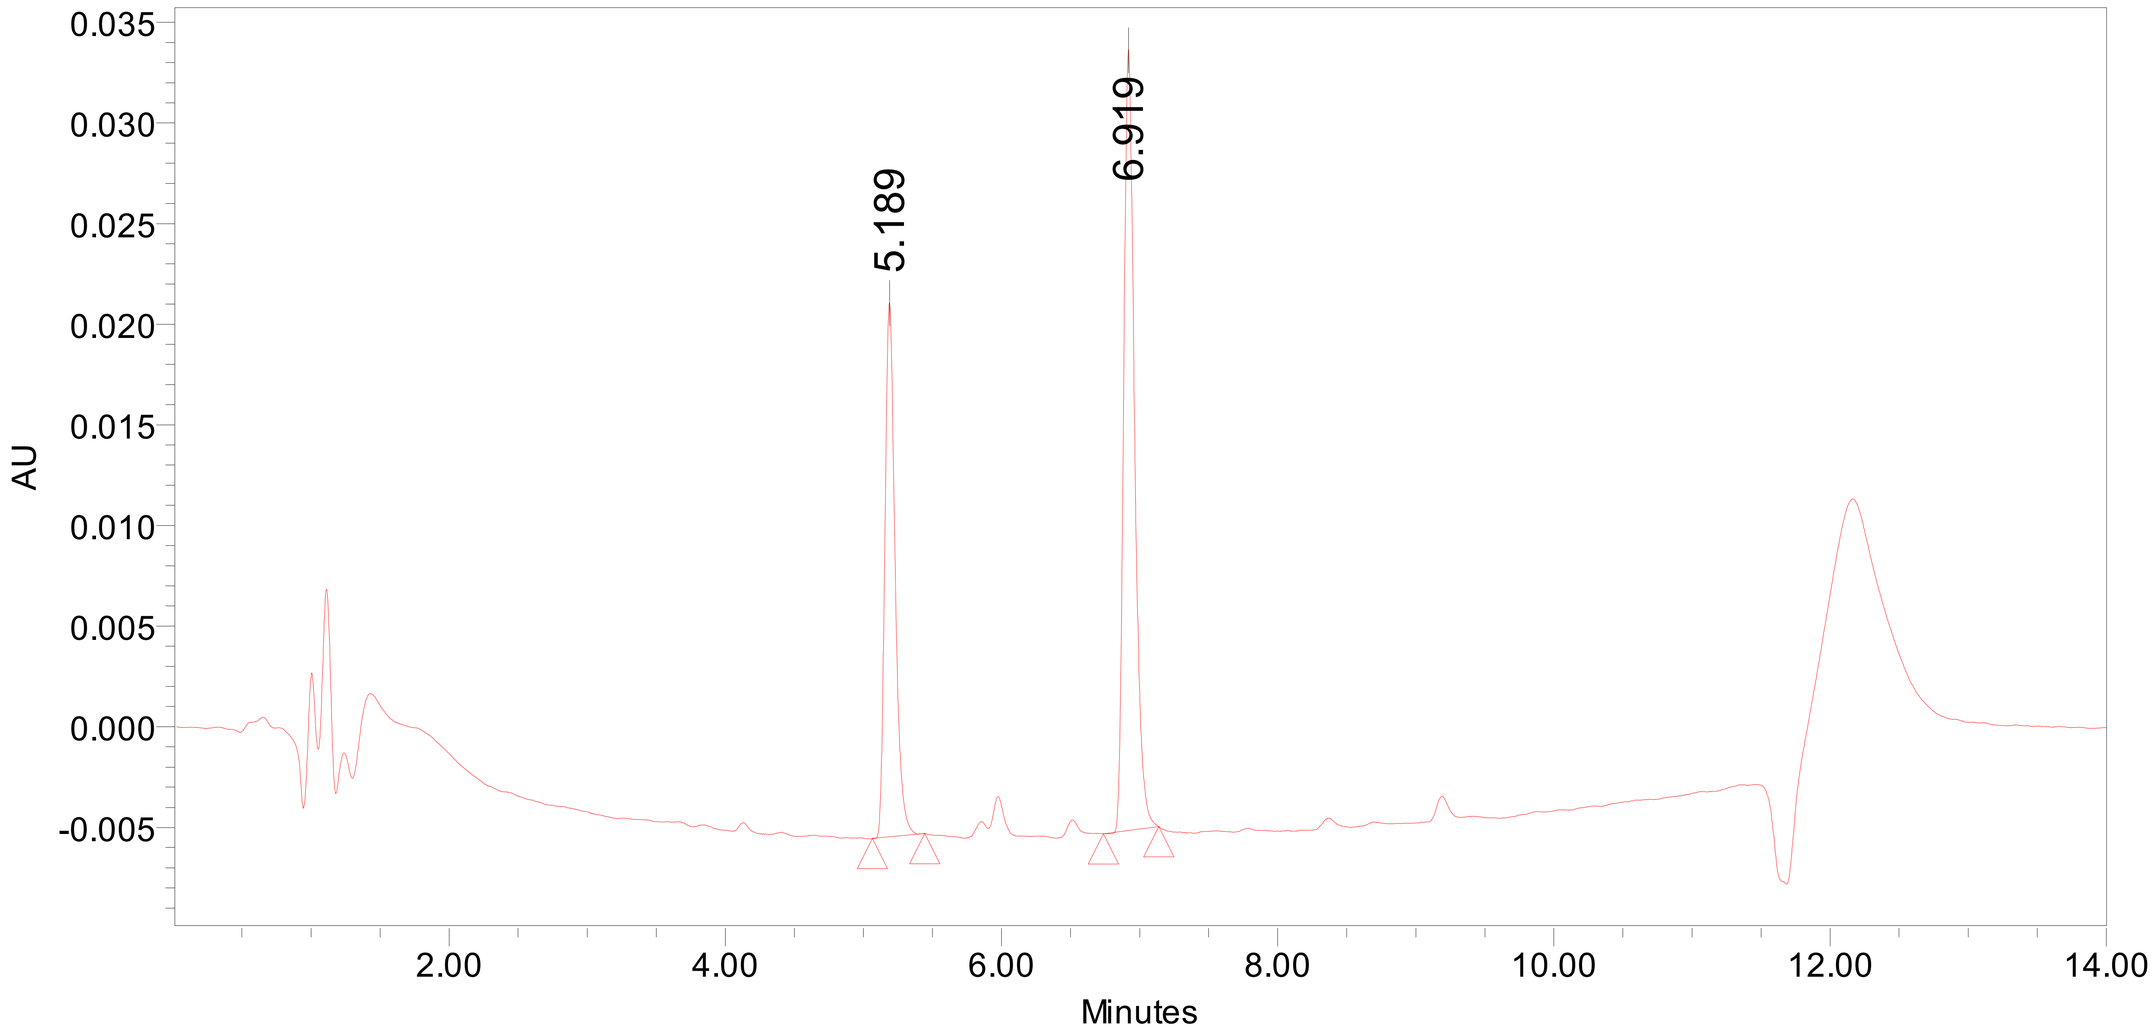

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.189	135907	26541		
2		6.919	215149	38803		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.189					
2		6.919					

SAMPLE INFORMATION

Sample Name:	HN170-Stability 1 day	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability 1 day
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-08 18:04:12 CET		
Date Processed:	2025-01-17 14:27:29 CET		

Auto-Scaled Chromatogram

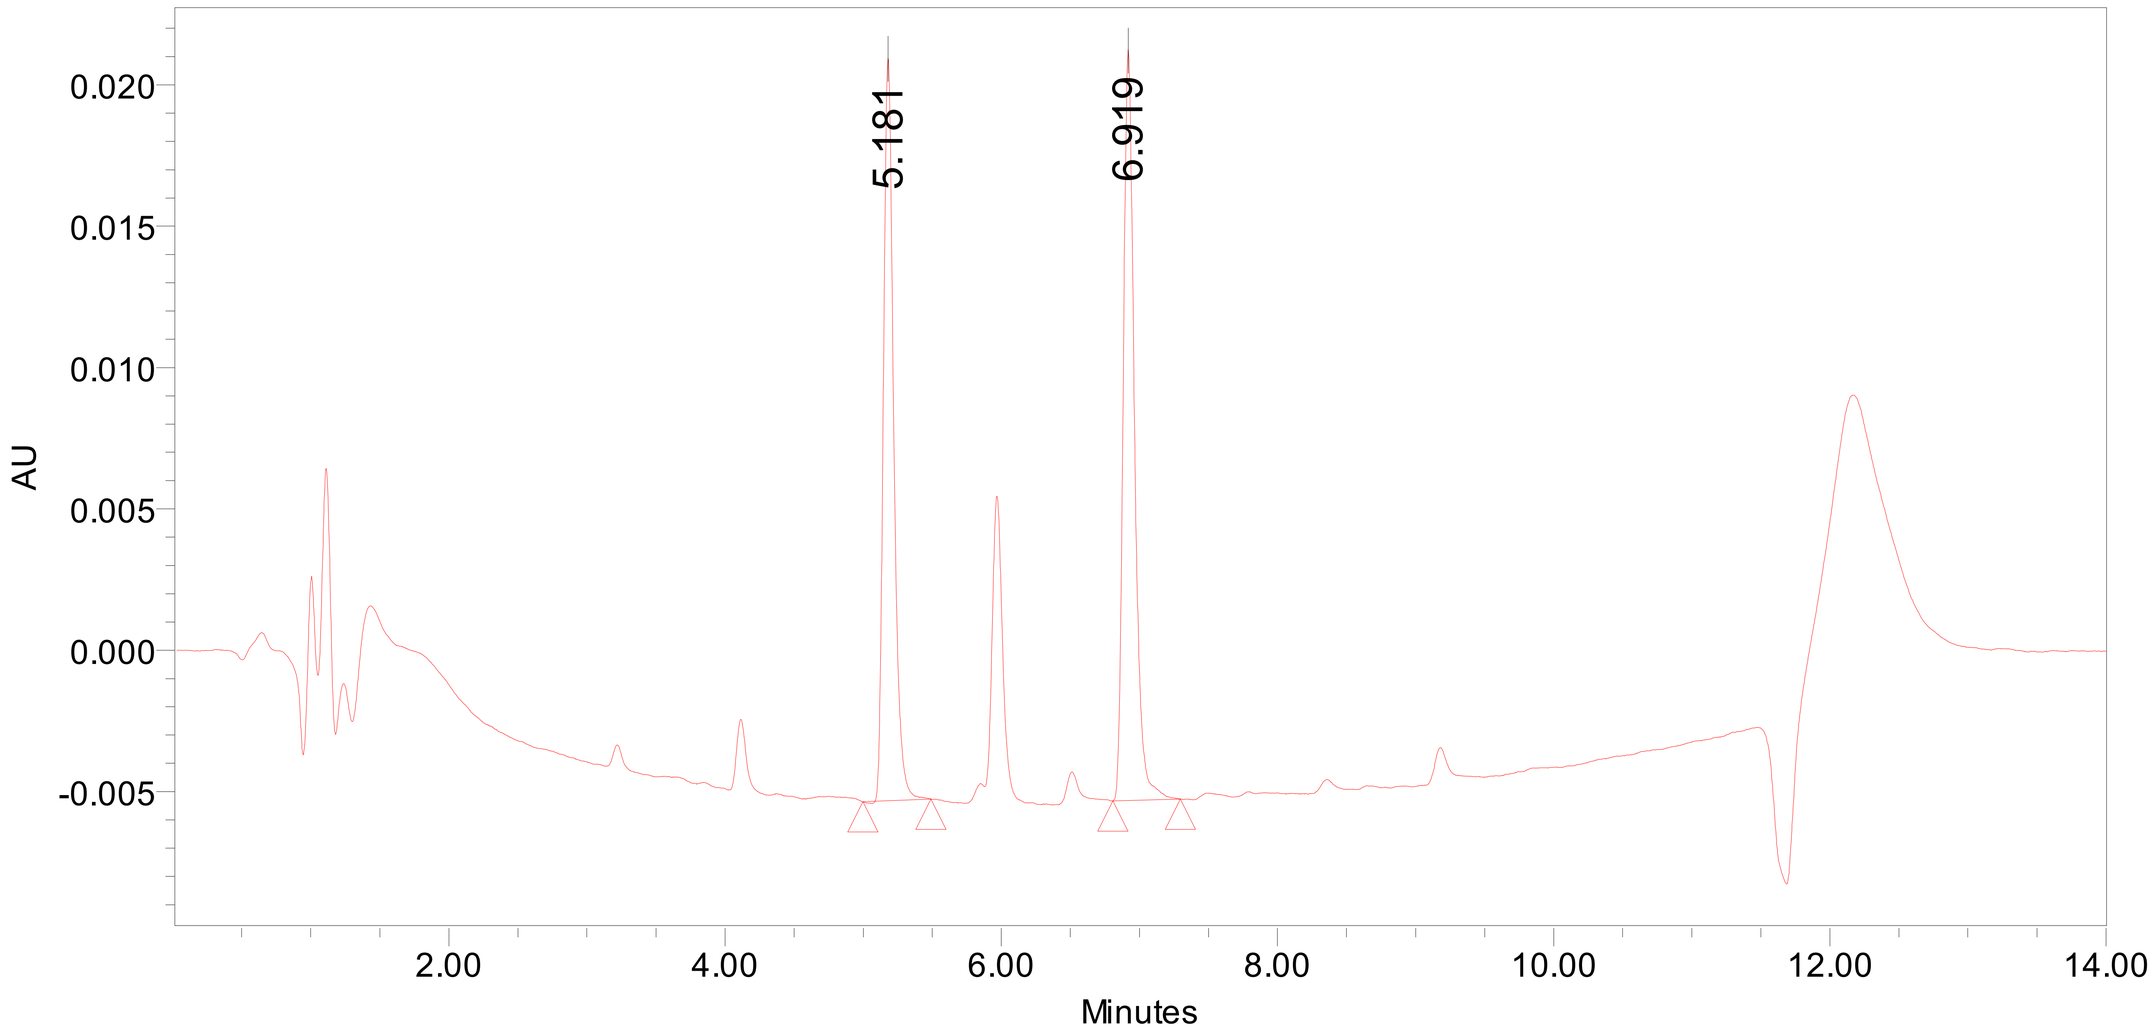

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.181	136315	26274		
2		6.919	151535	26566		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.181					
2		6.919					

SAMPLE INFORMATION

Sample Name:	HN170-Stability 2 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability 2 days
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-09 18:15:07 CET		
Date Processed:	2025-01-17 14:27:56 CET		

Auto-Scaled Chromatogram

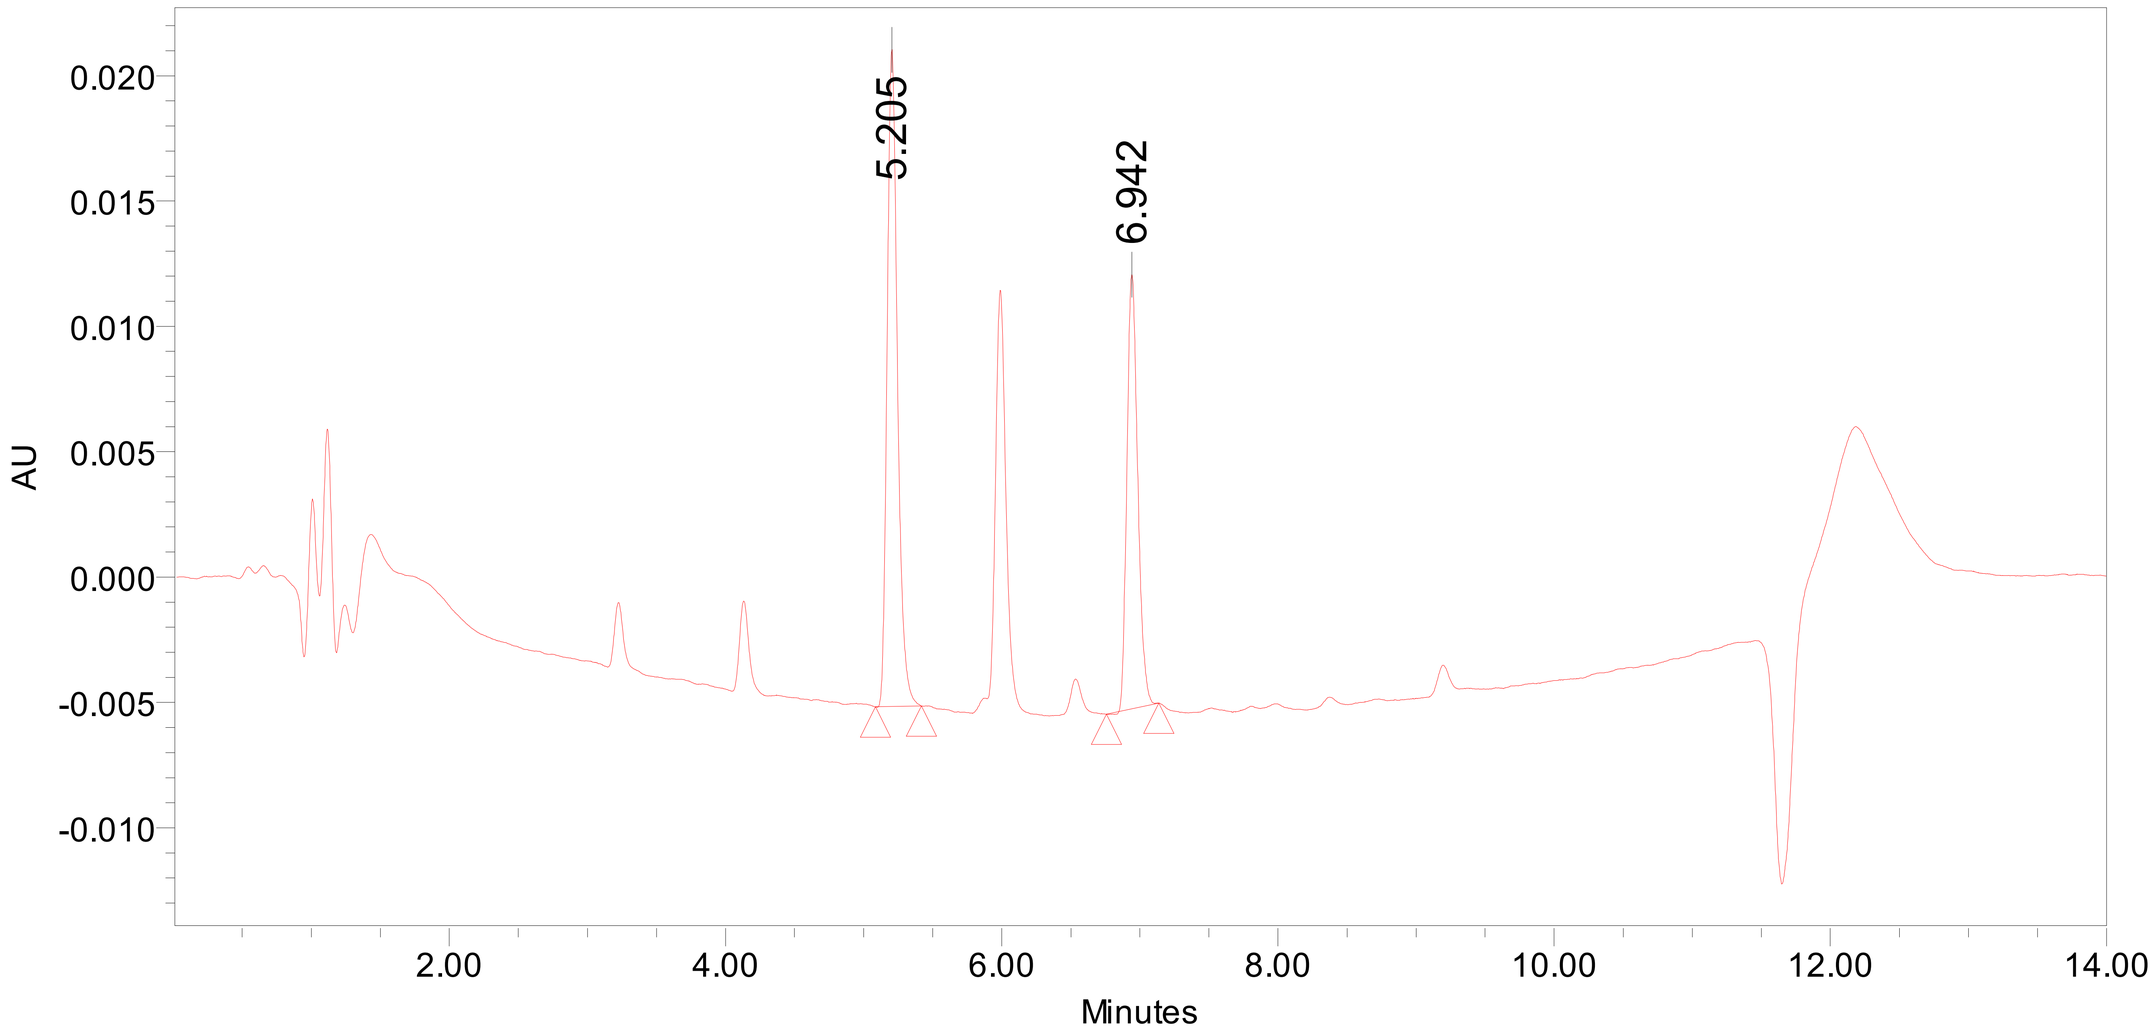

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.205	136019	26214		
2		6.942	95116	17322		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.205					
2		6.942					

SAMPLE INFORMATION

Sample Name:	HN170-Stability 3 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 3 days
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-10 17:51:03 CET		
Date Processed:	2025-01-17 14:28:21 CET		

Auto-Scaled Chromatogram

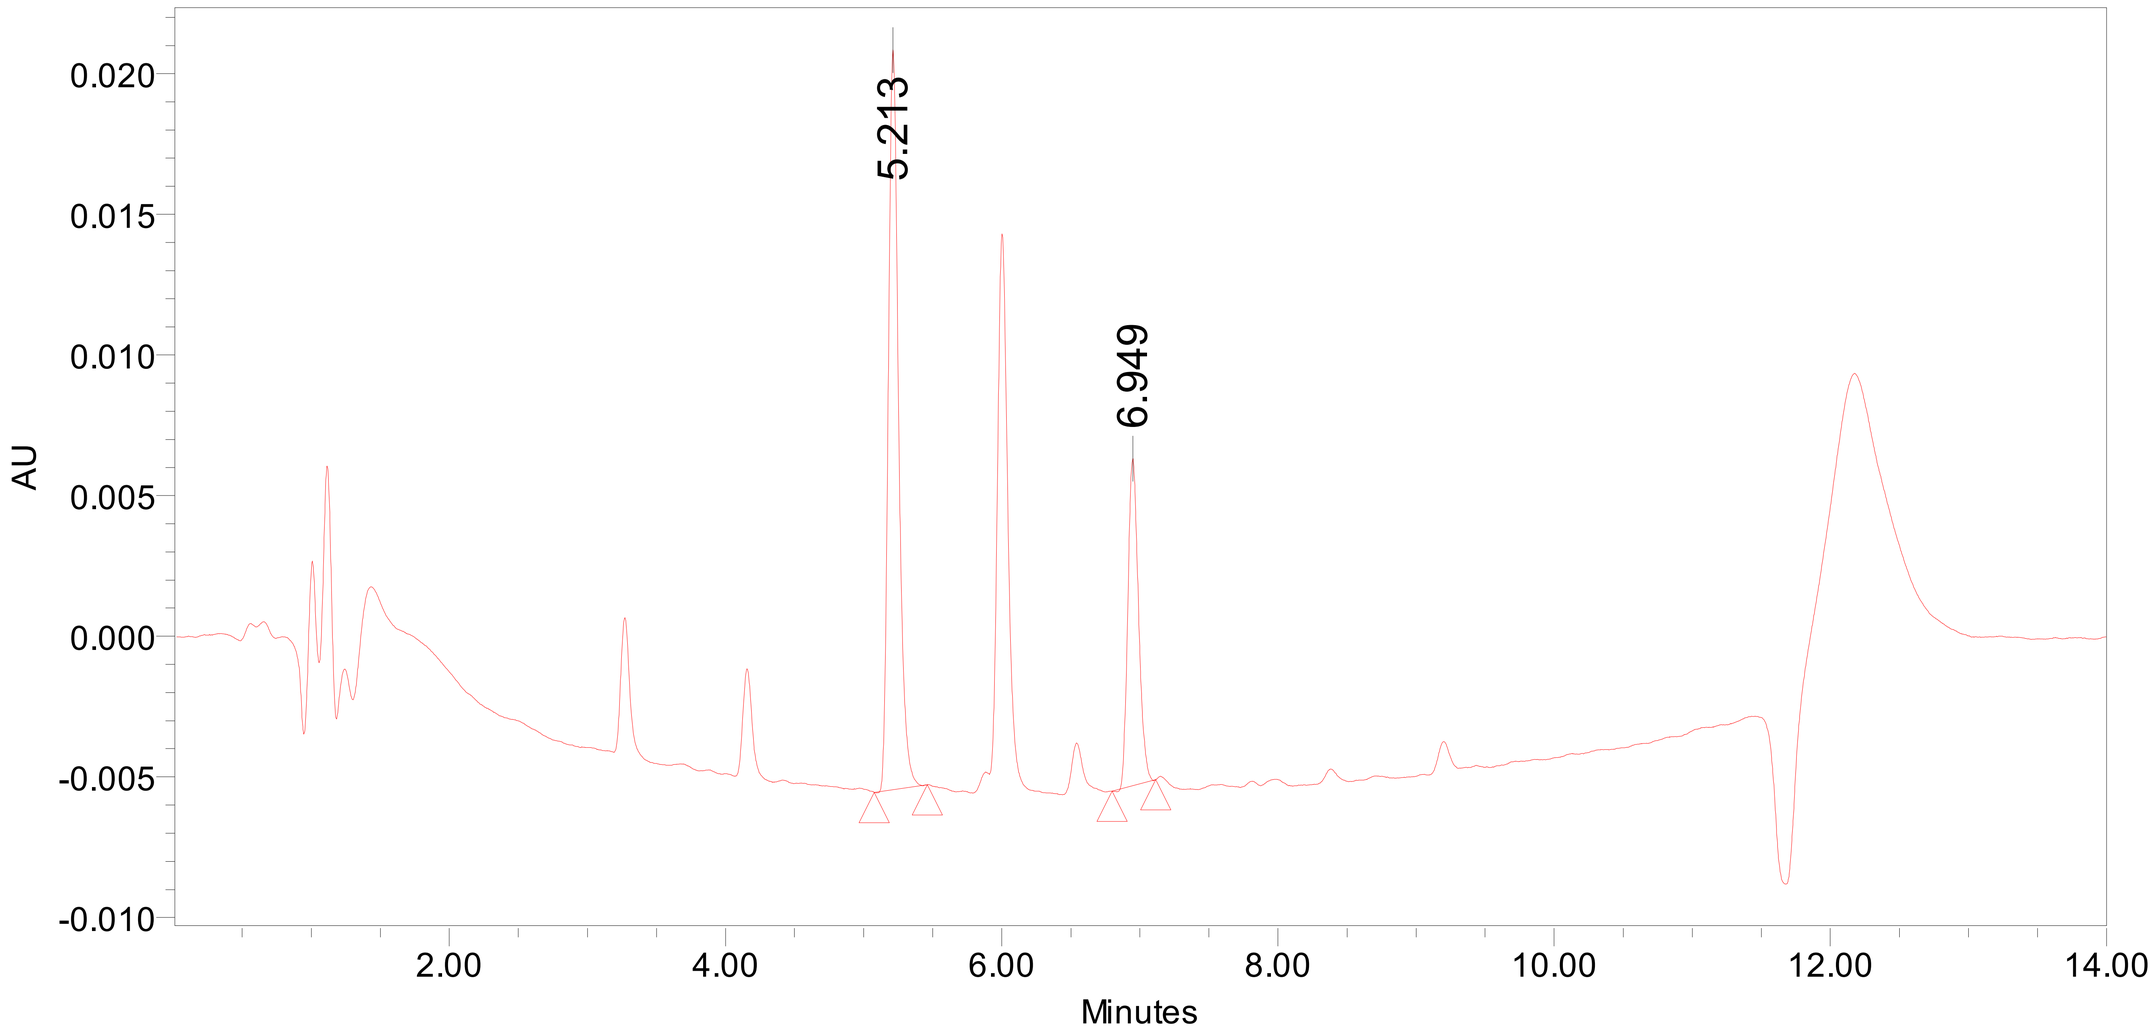

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.213	135404	26312		
2		6.949	62481	11627		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.213					
2		6.949					

SAMPLE INFORMATION

Sample Name:	HN170-Stability 4 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 4 days
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-11 14:35:03 CET		
Date Processed:	2025-01-17 14:28:40 CET		

Auto-Scaled Chromatogram

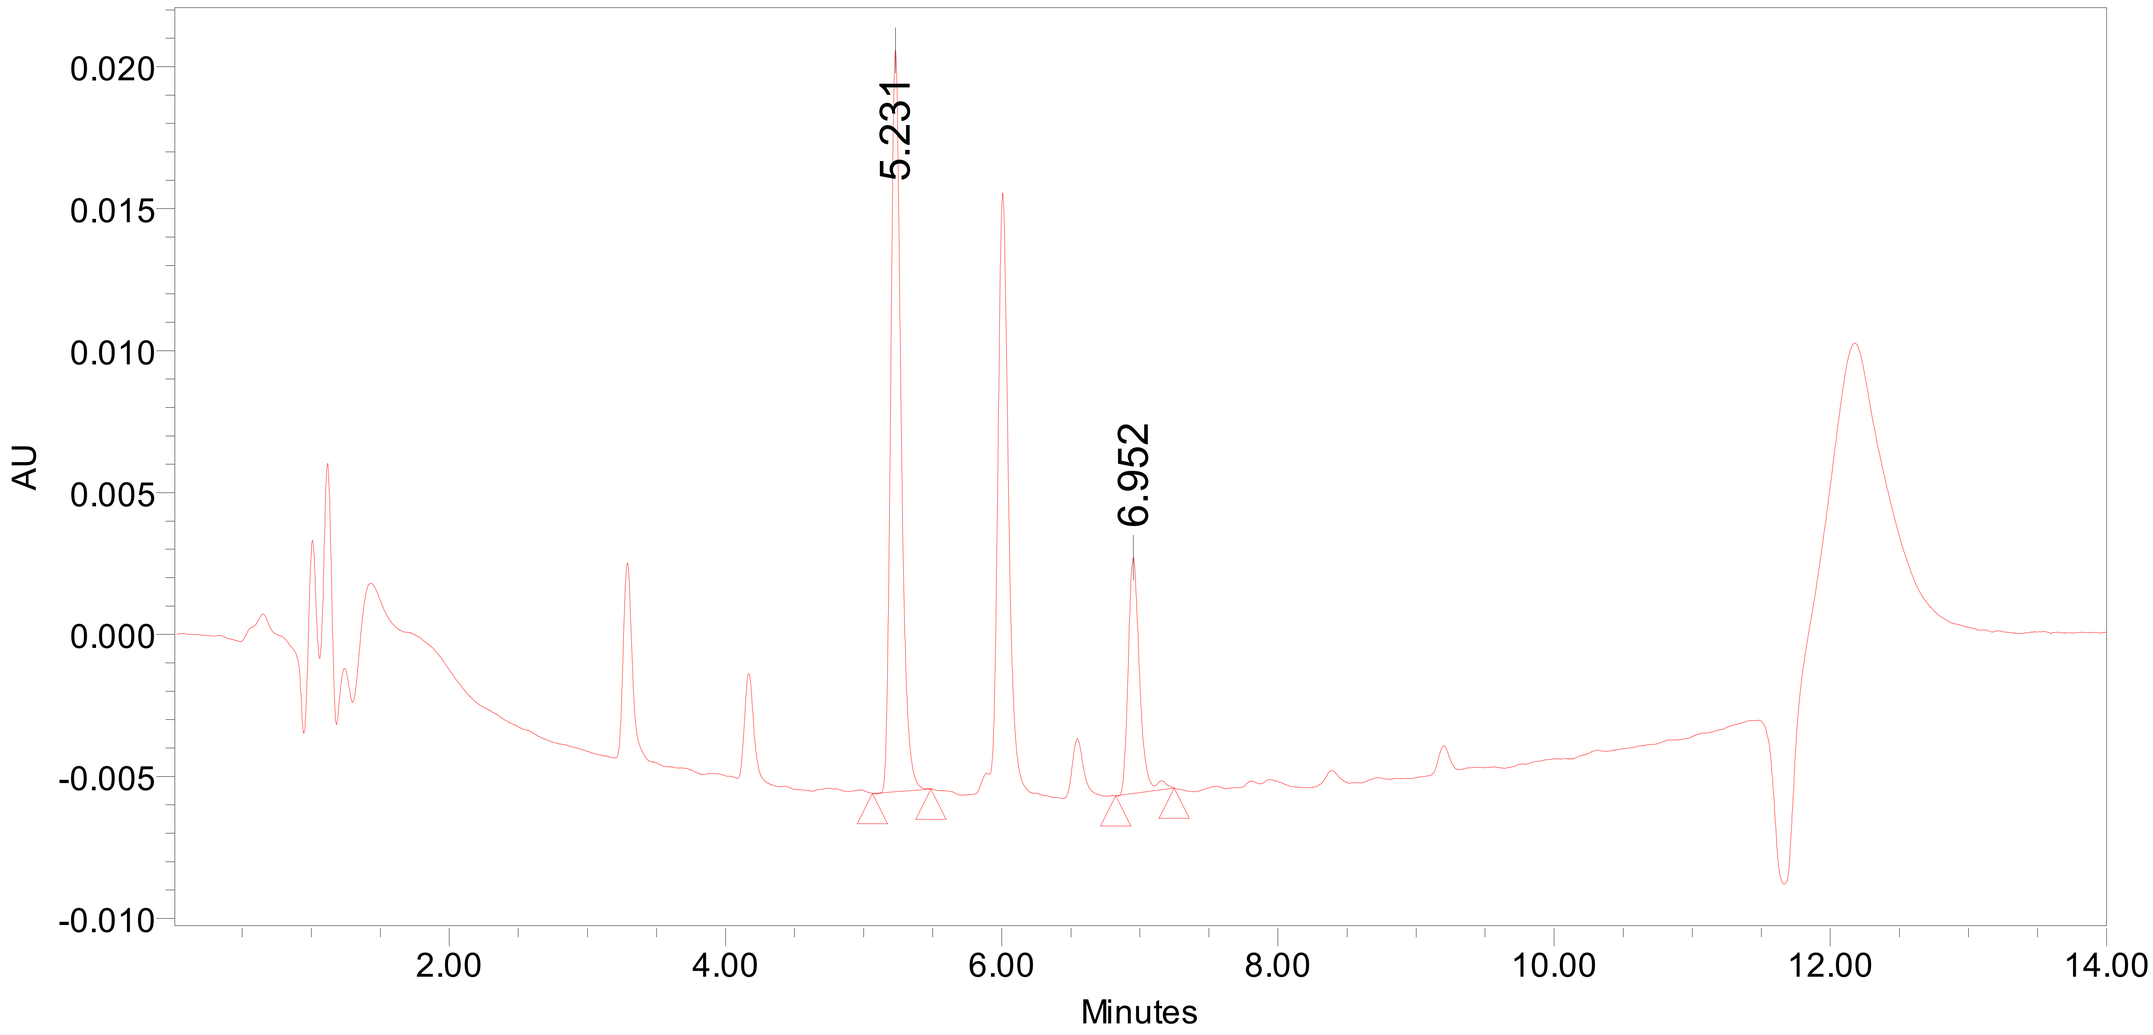

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.231	135492	26151		
2		6.952	47875	8311		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.231					
2		6.952					

SAMPLE INFORMATION

Sample Name:	HN170-Stability 6 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability 6 days
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-13 12:52:12 CET		
Date Processed:	2025-01-17 14:29:02 CET		

Auto-Scaled Chromatogram

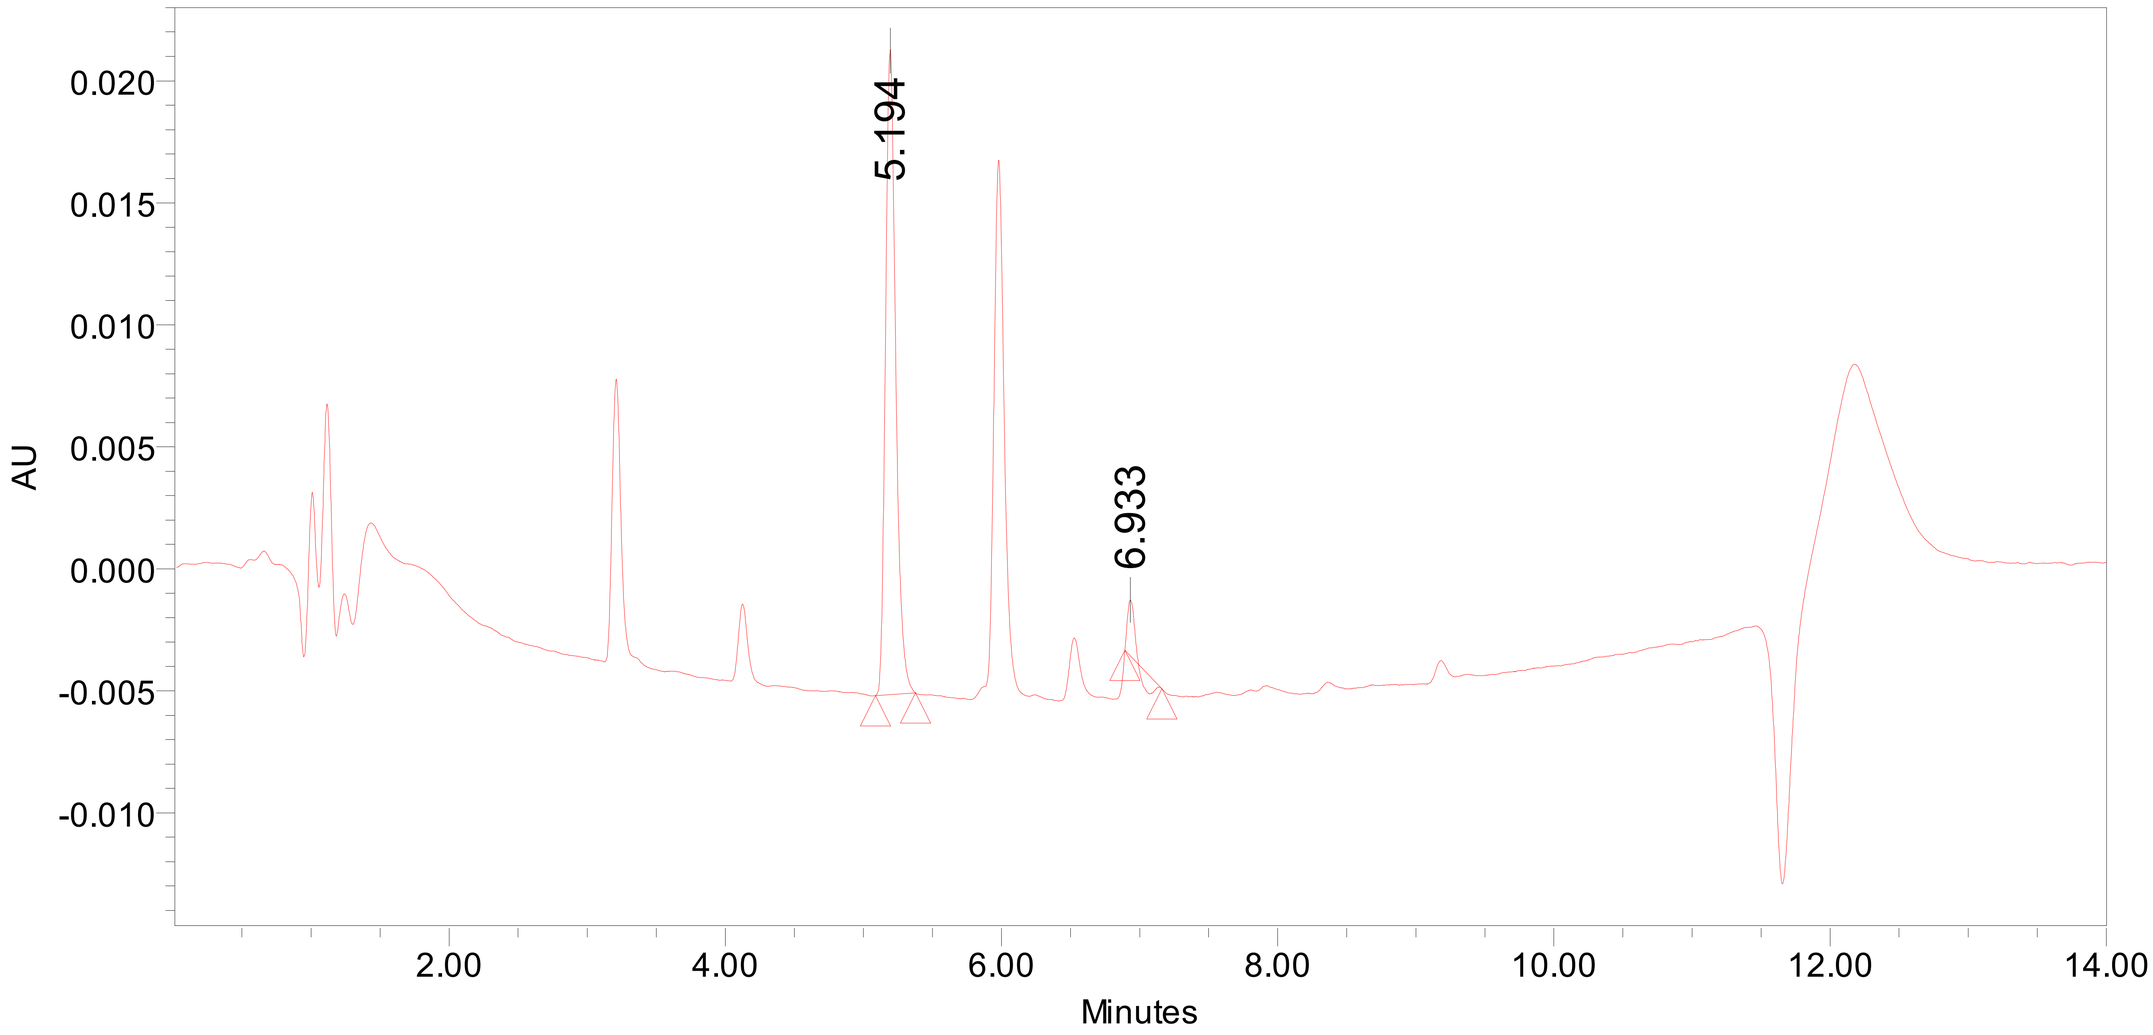

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.194	135859	26442		
2		6.933	12593	2295		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.194					
2		6.933					

SAMPLE INFORMATION

Sample Name:	HN170-Stability 7 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 7 days
Vial:	11	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-14 15:32:10 CET		
Date Processed:	2025-01-17 14:29:26 CET		

Auto-Scaled Chromatogram

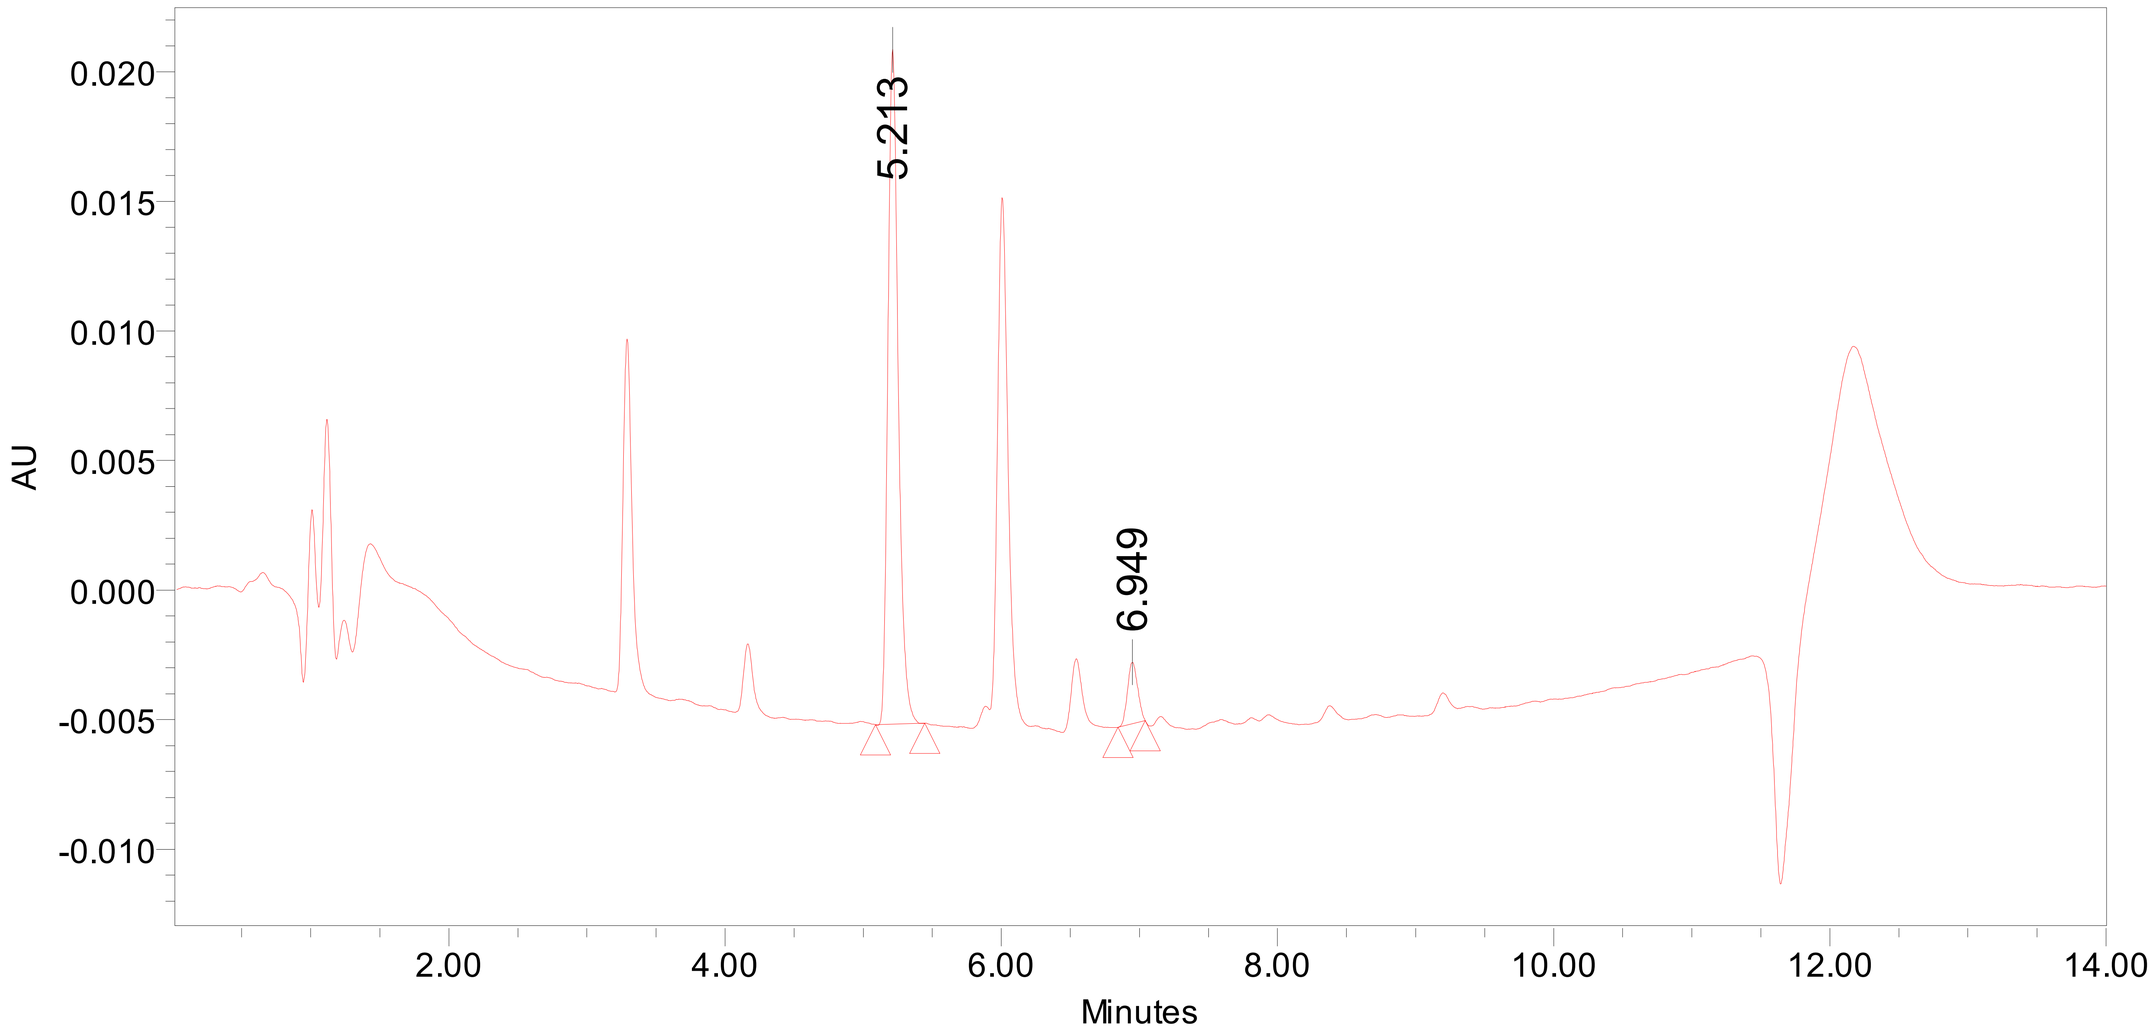

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.213	135254	26034		
2		6.949	12028	2363		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.213					
2		6.949					