
SAMPLE INFORMATION

Sample Name:	Hk13-Stability 2-time 0	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability repeat time 0
Vial:	104	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-15 13:22:51 CET		
Date Processed:	2025-01-20 14:35:02 CET		

Auto-Scaled Chromatogram

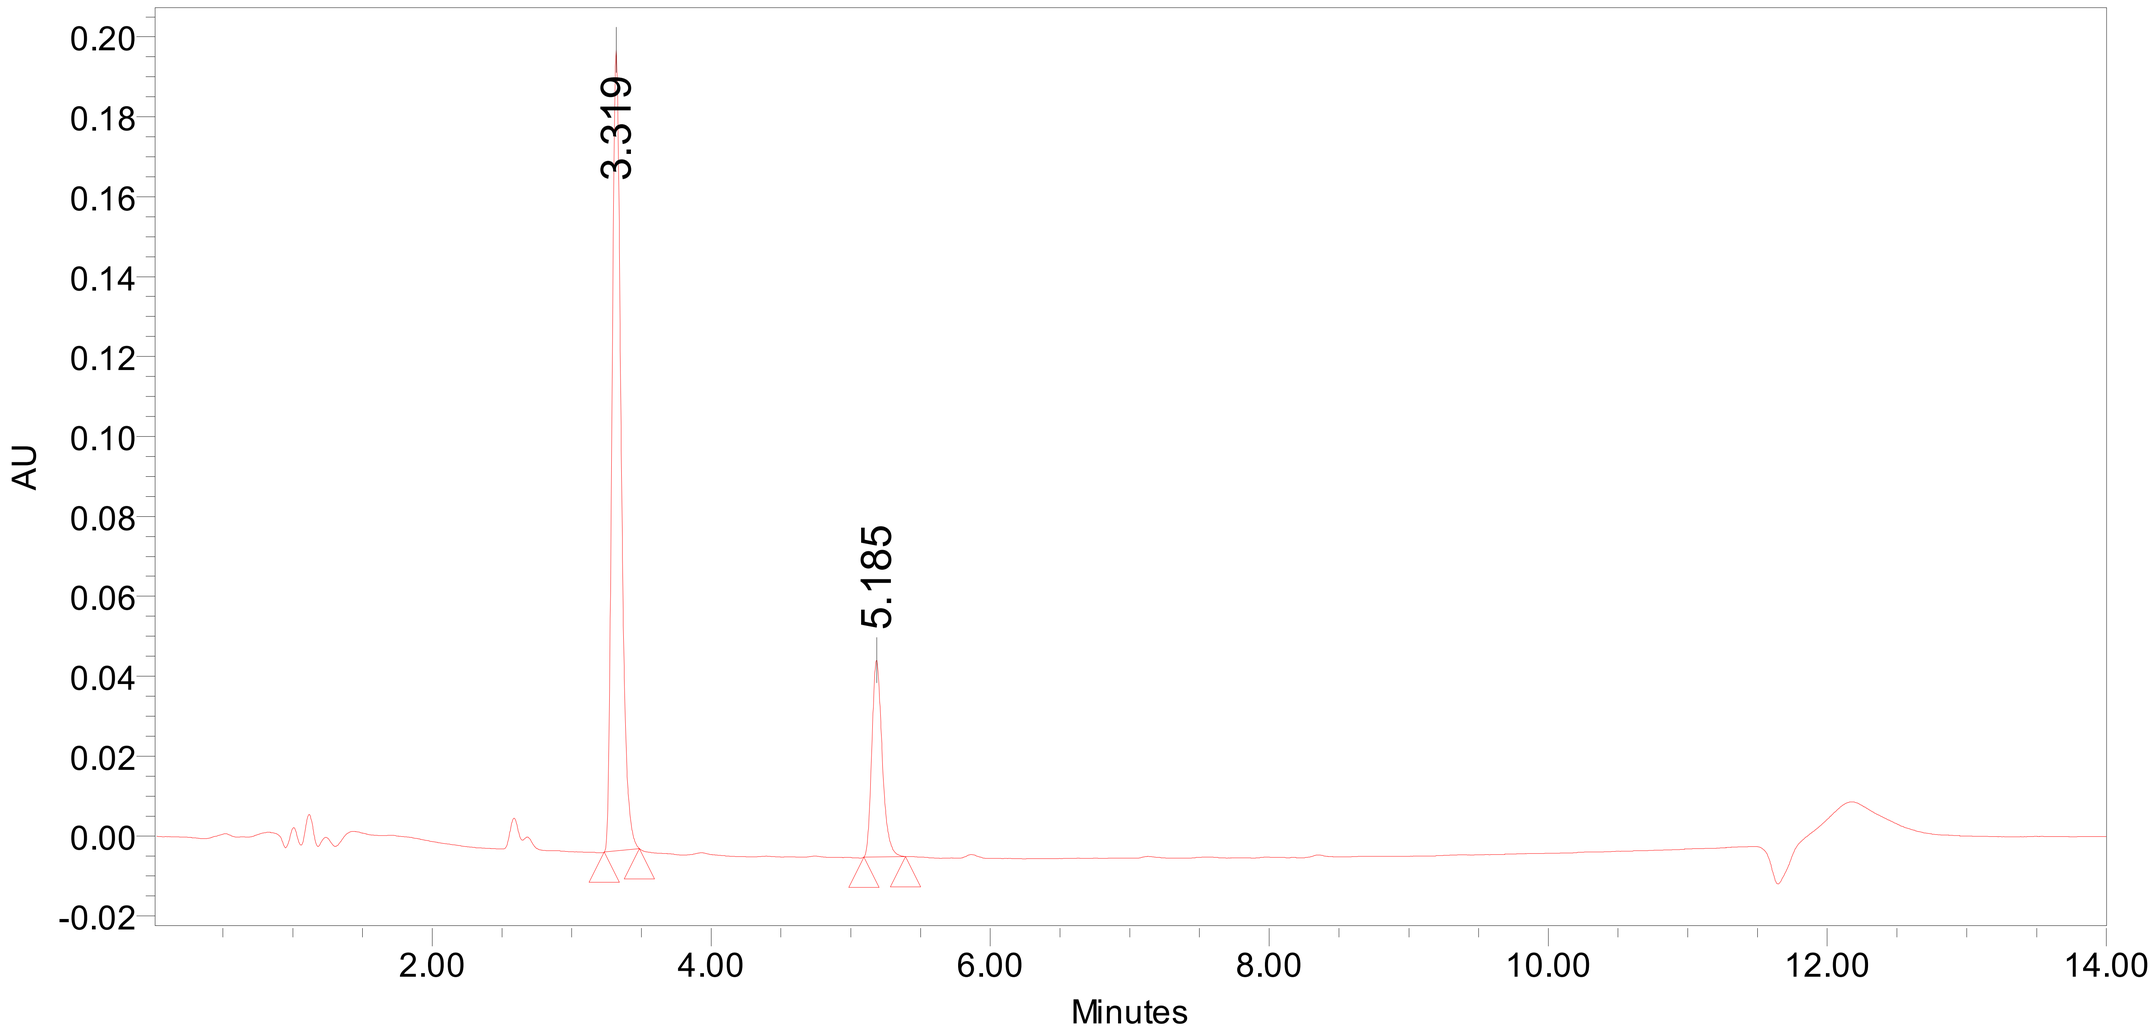

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.319	905462	200595		
2		5.185	254597	49261		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.319					
2		5.185					

SAMPLE INFORMATION

Sample Name:	HK13-Stability repeat-1 day	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability repeat 1 day
Vial:	104	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-16 16:04:05 CET		
Date Processed:	2025-01-20 14:35:17 CET		

Auto-Scaled Chromatogram

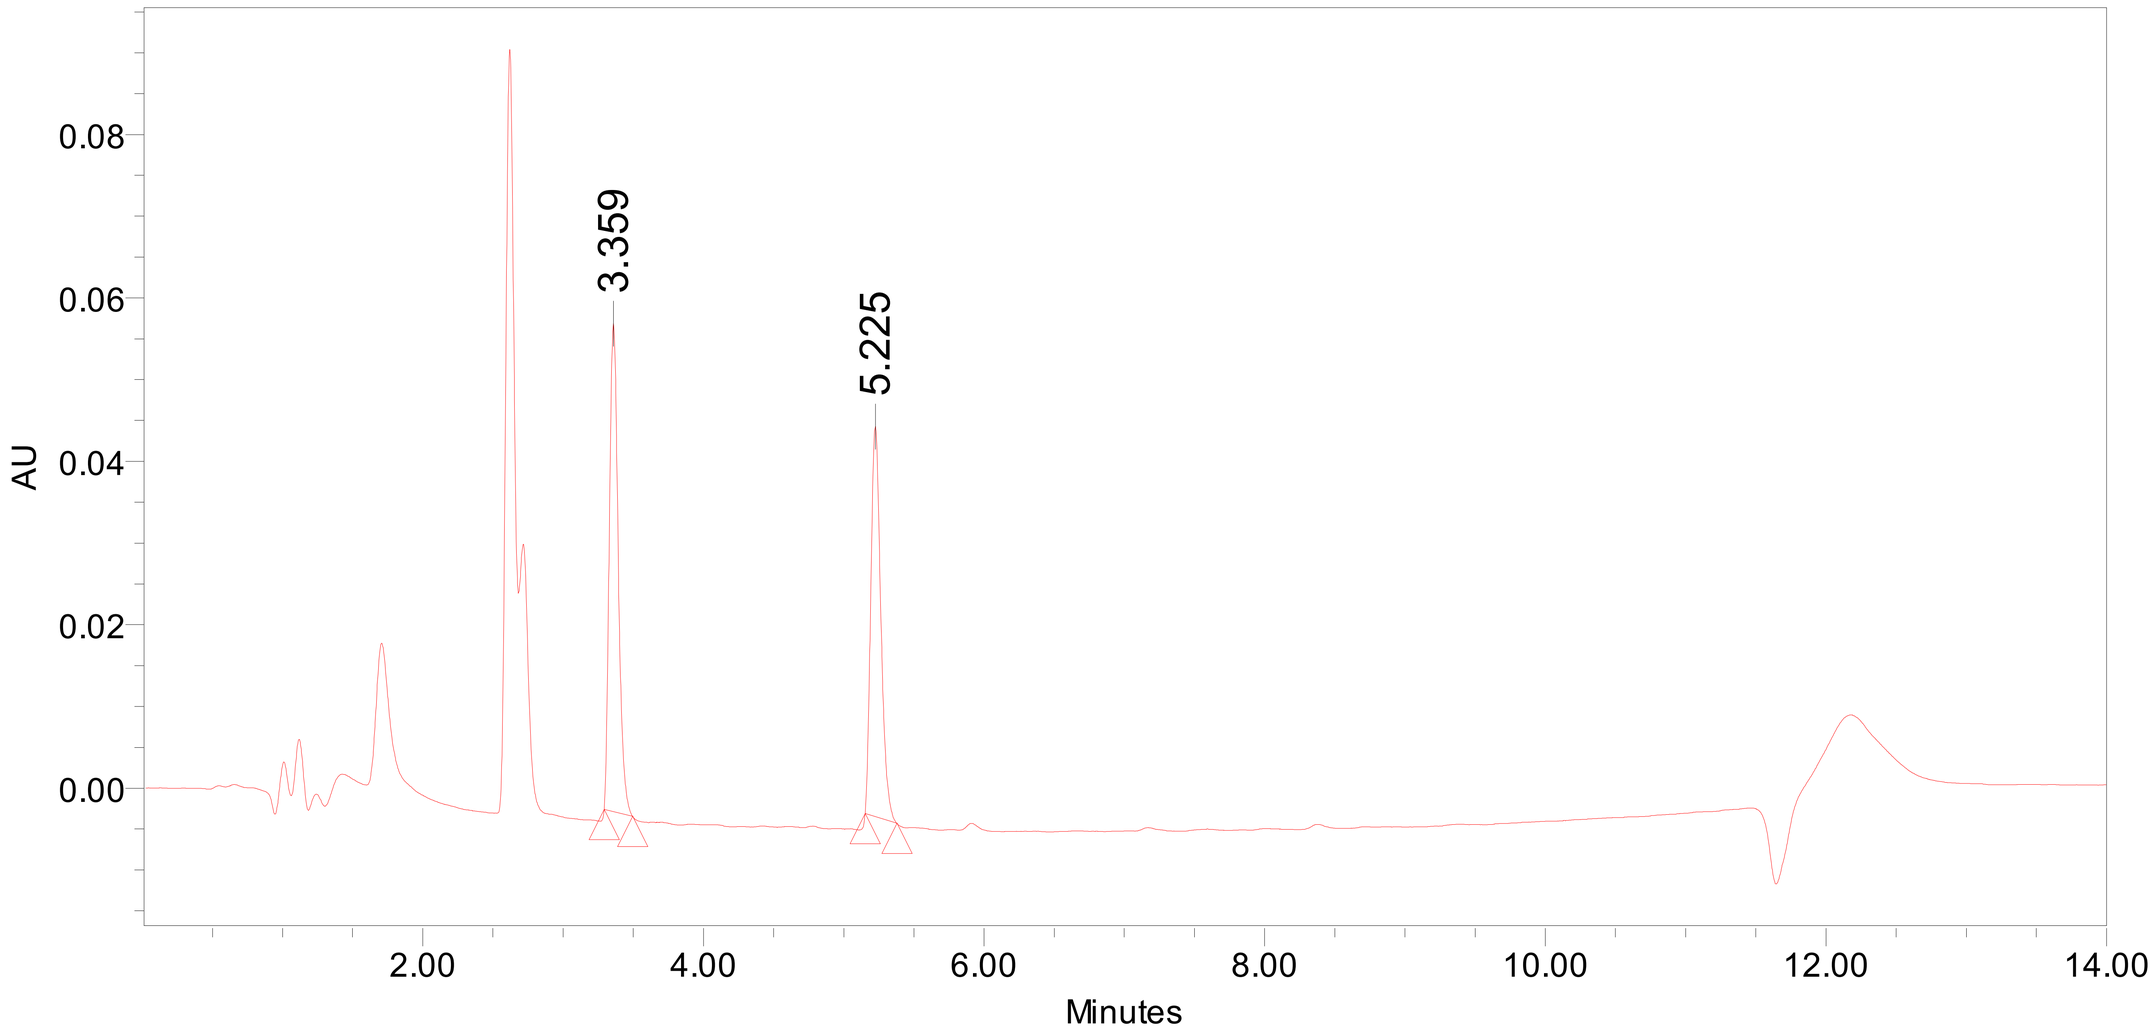

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.359	261809	59770		
2		5.225	237335	47738		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.359					
2		5.225					

SAMPLE INFORMATION

Sample Name:	HK13-Stability repeat-2 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability repeat 2 days
Vial:	104	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-17 18:00:40 CET		
Date Processed:	2025-01-20 14:35:43 CET		

Auto-Scaled Chromatogram

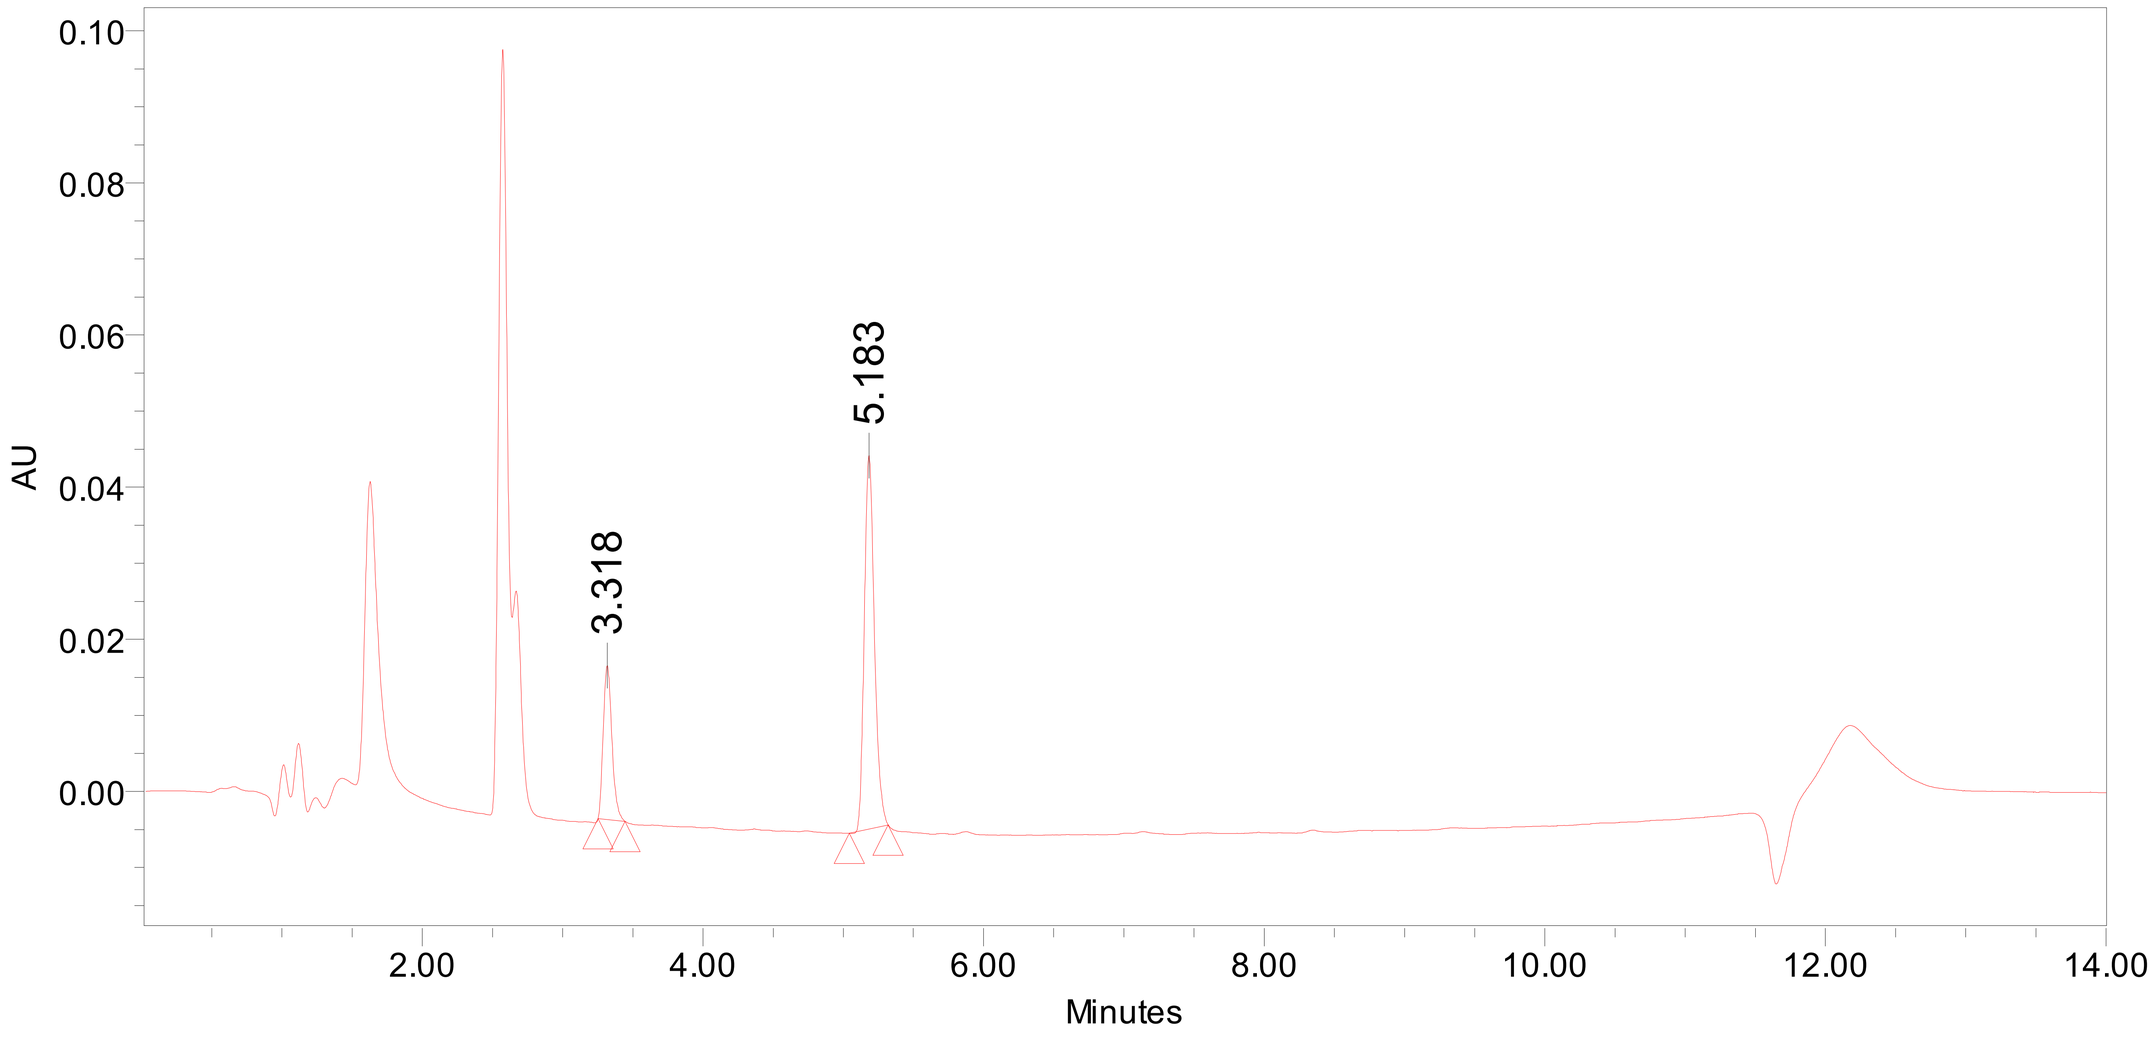

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.318	87875	20233		
2		5.183	247252	49103		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.318					
2		5.183					

SAMPLE INFORMATION

Sample Name:	HK13-Stability repeat-3 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability repeat 3 days
Vial:	104	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-18 18:09:00 CET		
Date Processed:	2025-01-20 14:36:00 CET		

Auto-Scaled Chromatogram

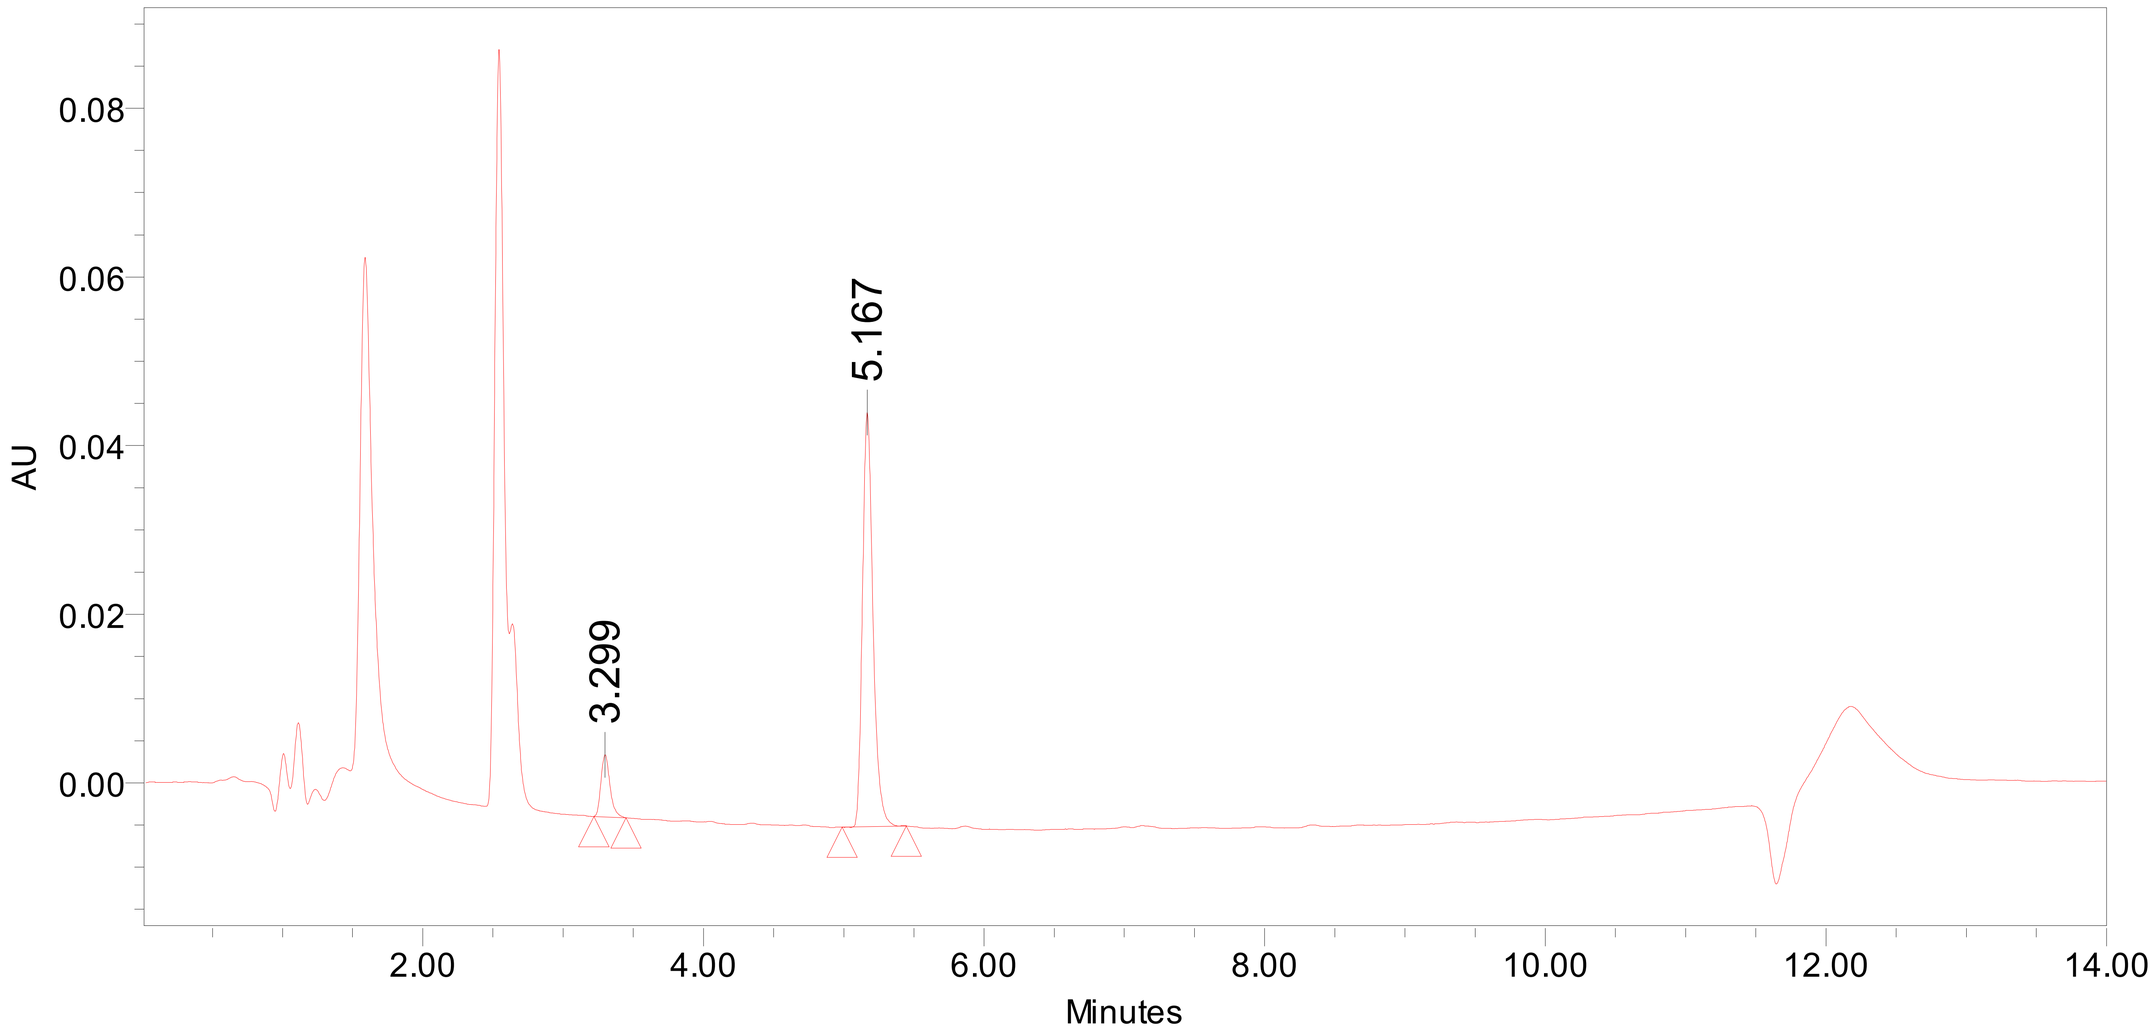

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.299	33206	7368		
2		5.167	256827	49149		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.299					
2		5.167					

SAMPLE INFORMATION

Sample Name:	HK13-Stability repeat-4 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 4 days
Vial:	104	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-19 17:30:13 CET		
Date Processed:	2025-01-20 14:36:39 CET		

Auto-Scaled Chromatogram

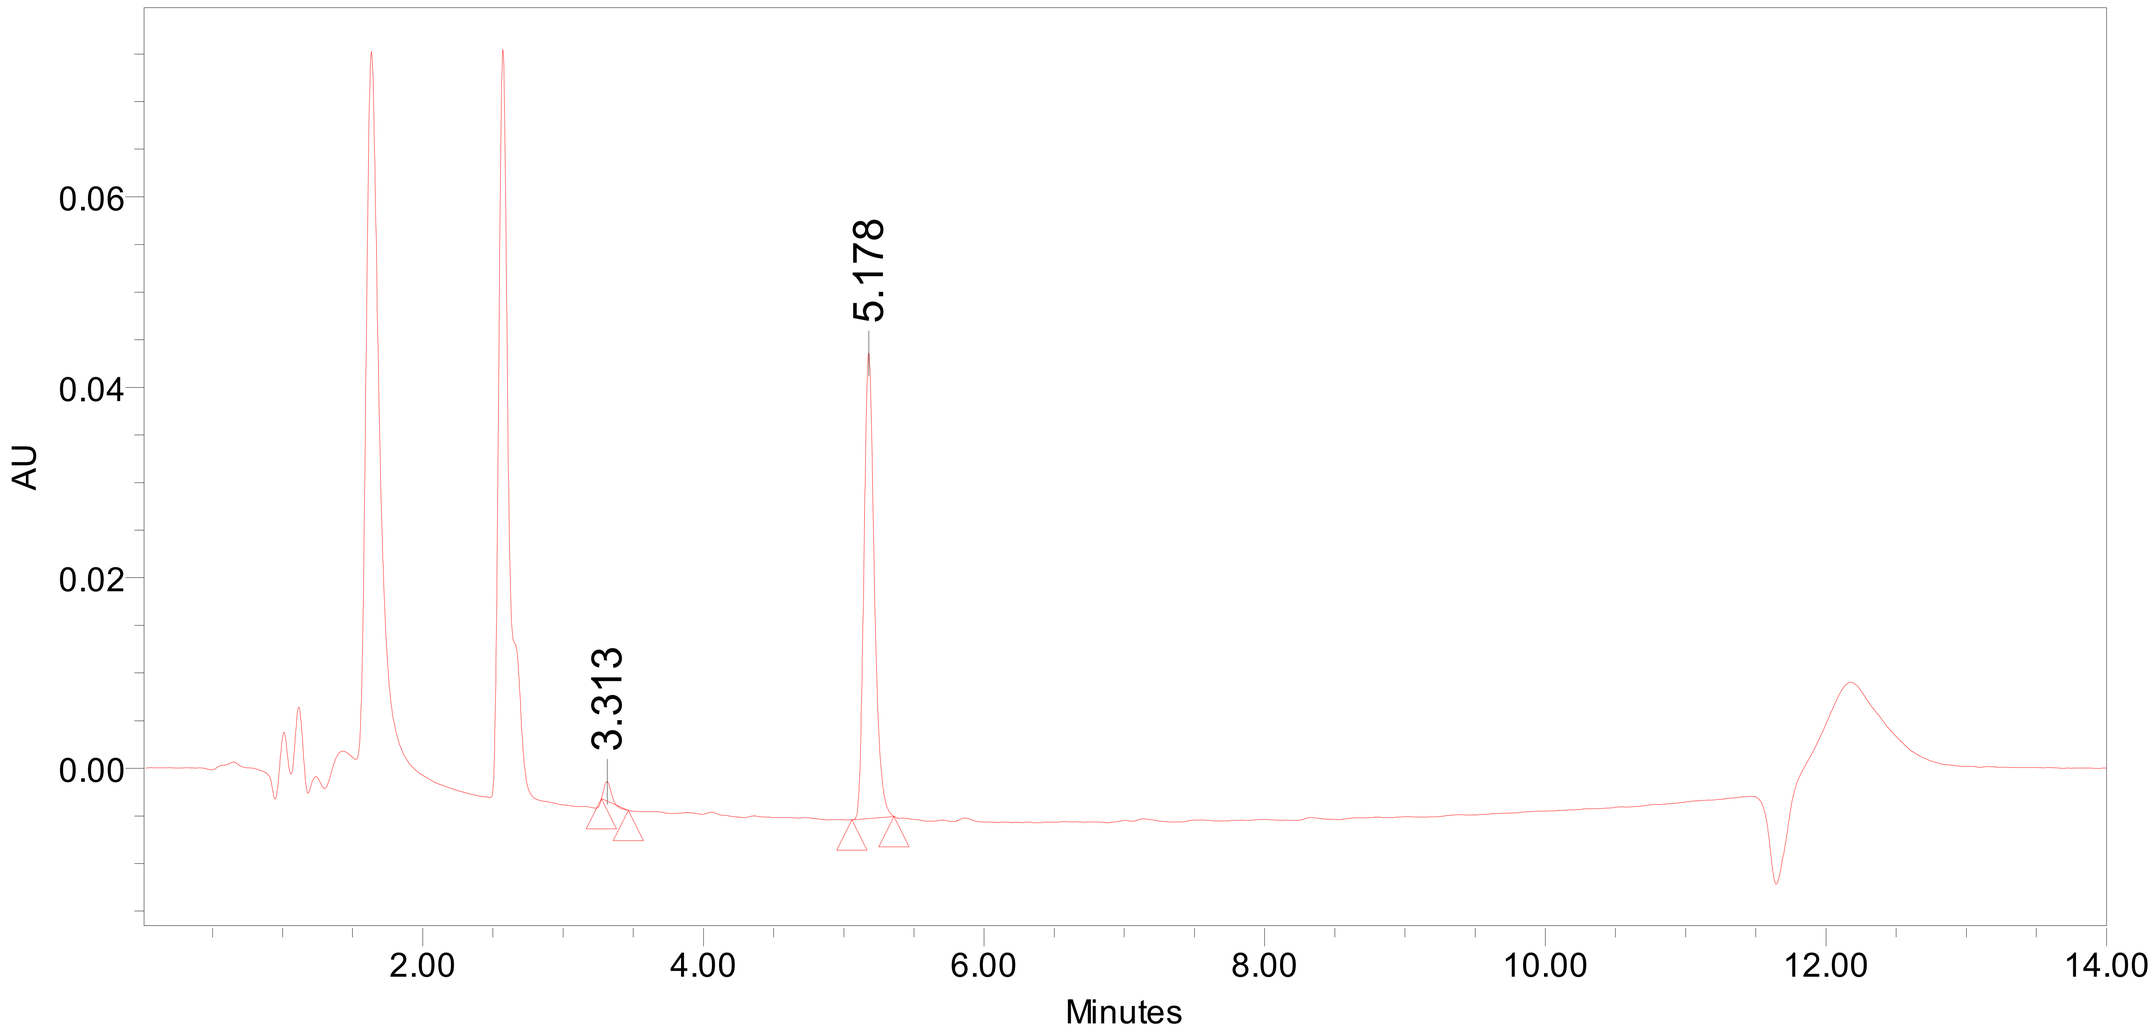

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.313	7354	2053		
2		5.178	254454	48928		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.313					
2		5.178					