
SAMPLE INFORMATION

Sample Name:	AV407-Blank	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 av407 blanks
Vial:	71	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-23 15:46:32 CET		
Date Processed:	2025-02-04 14:49:45 CET		

Auto-Scaled Chromatogram

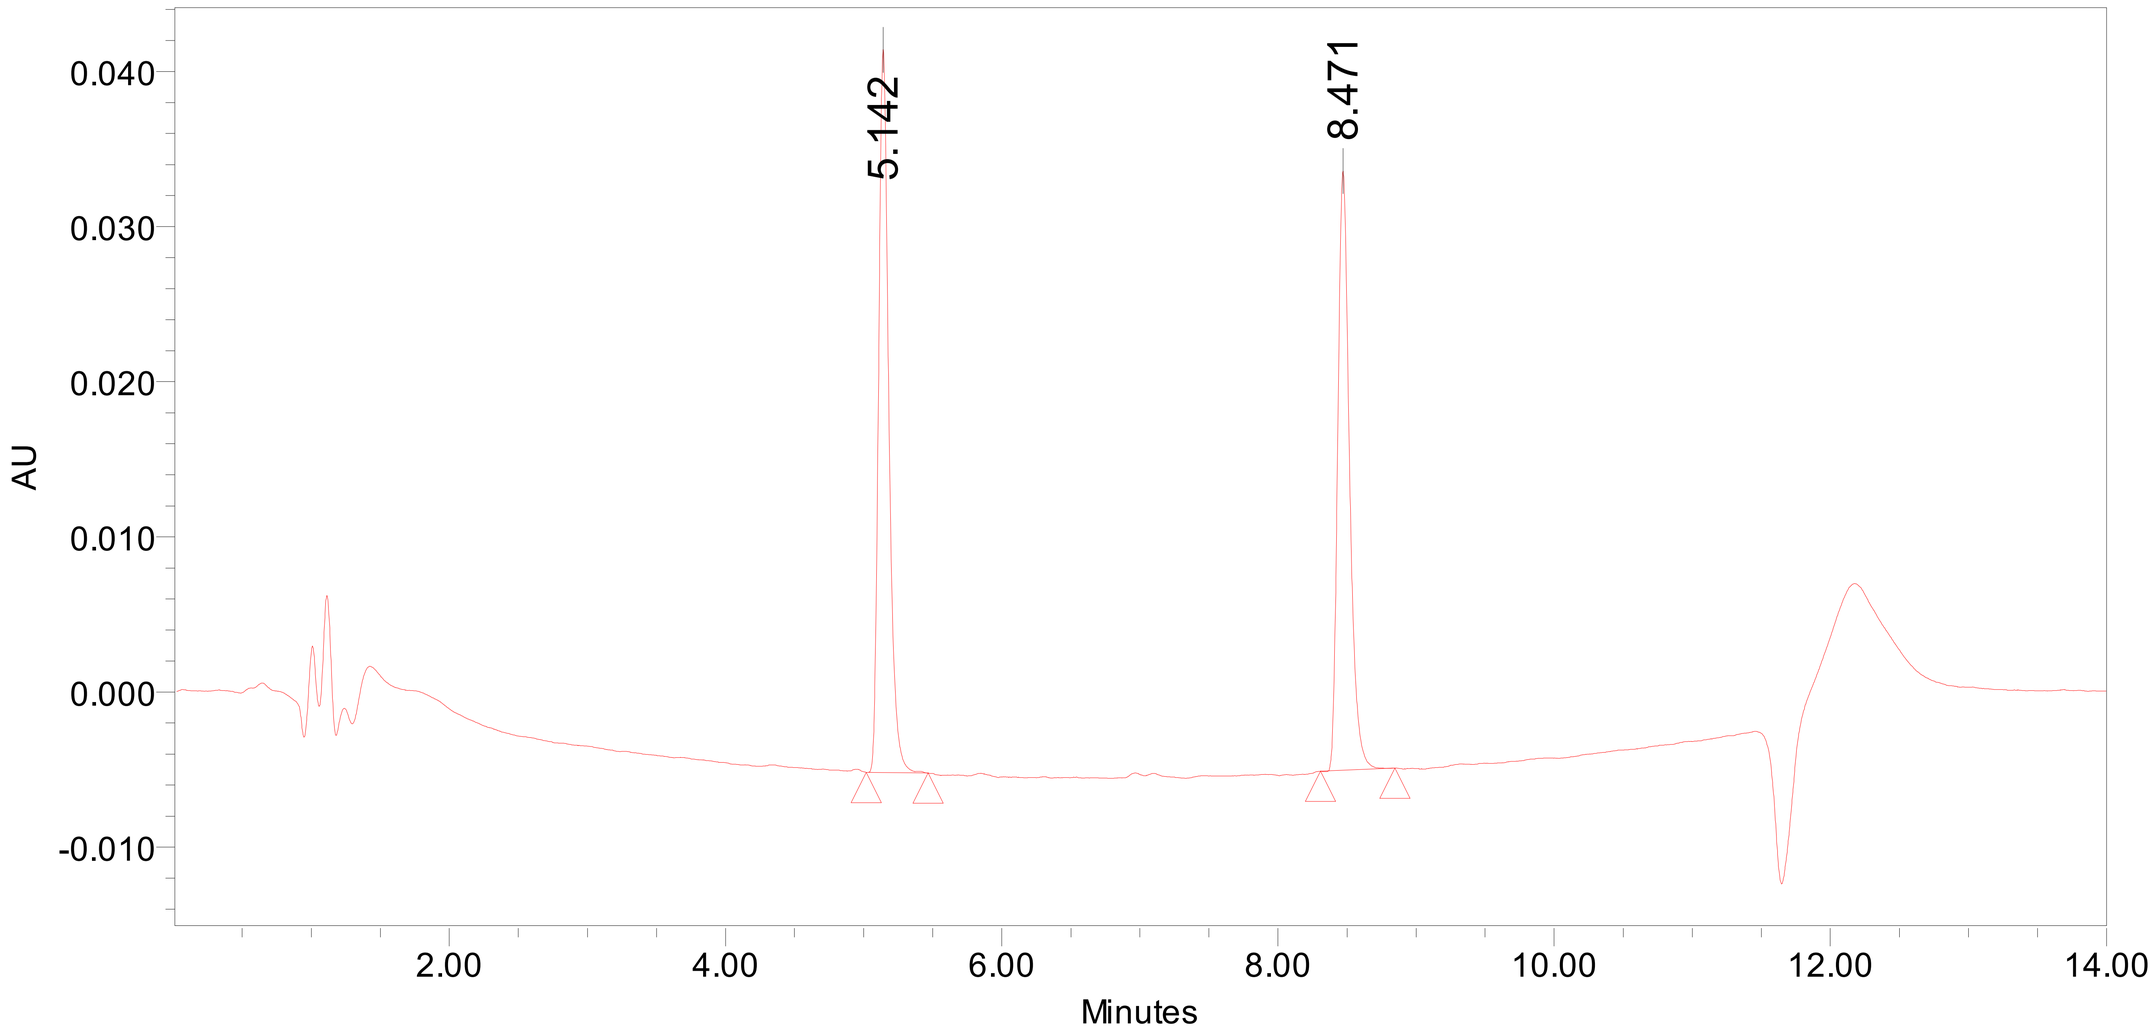

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.142	241368	46602		
2		8.471	229380	38636		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.142					
2		8.471					

SAMPLE INFORMATION

Sample Name:	AV407-Stability-1 day	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 av407 av422 stab 1 day
Vial:	71	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-24 13:09:51 CET		
Date Processed:	2025-02-04 14:47:50 CET		

Auto-Scaled Chromatogram

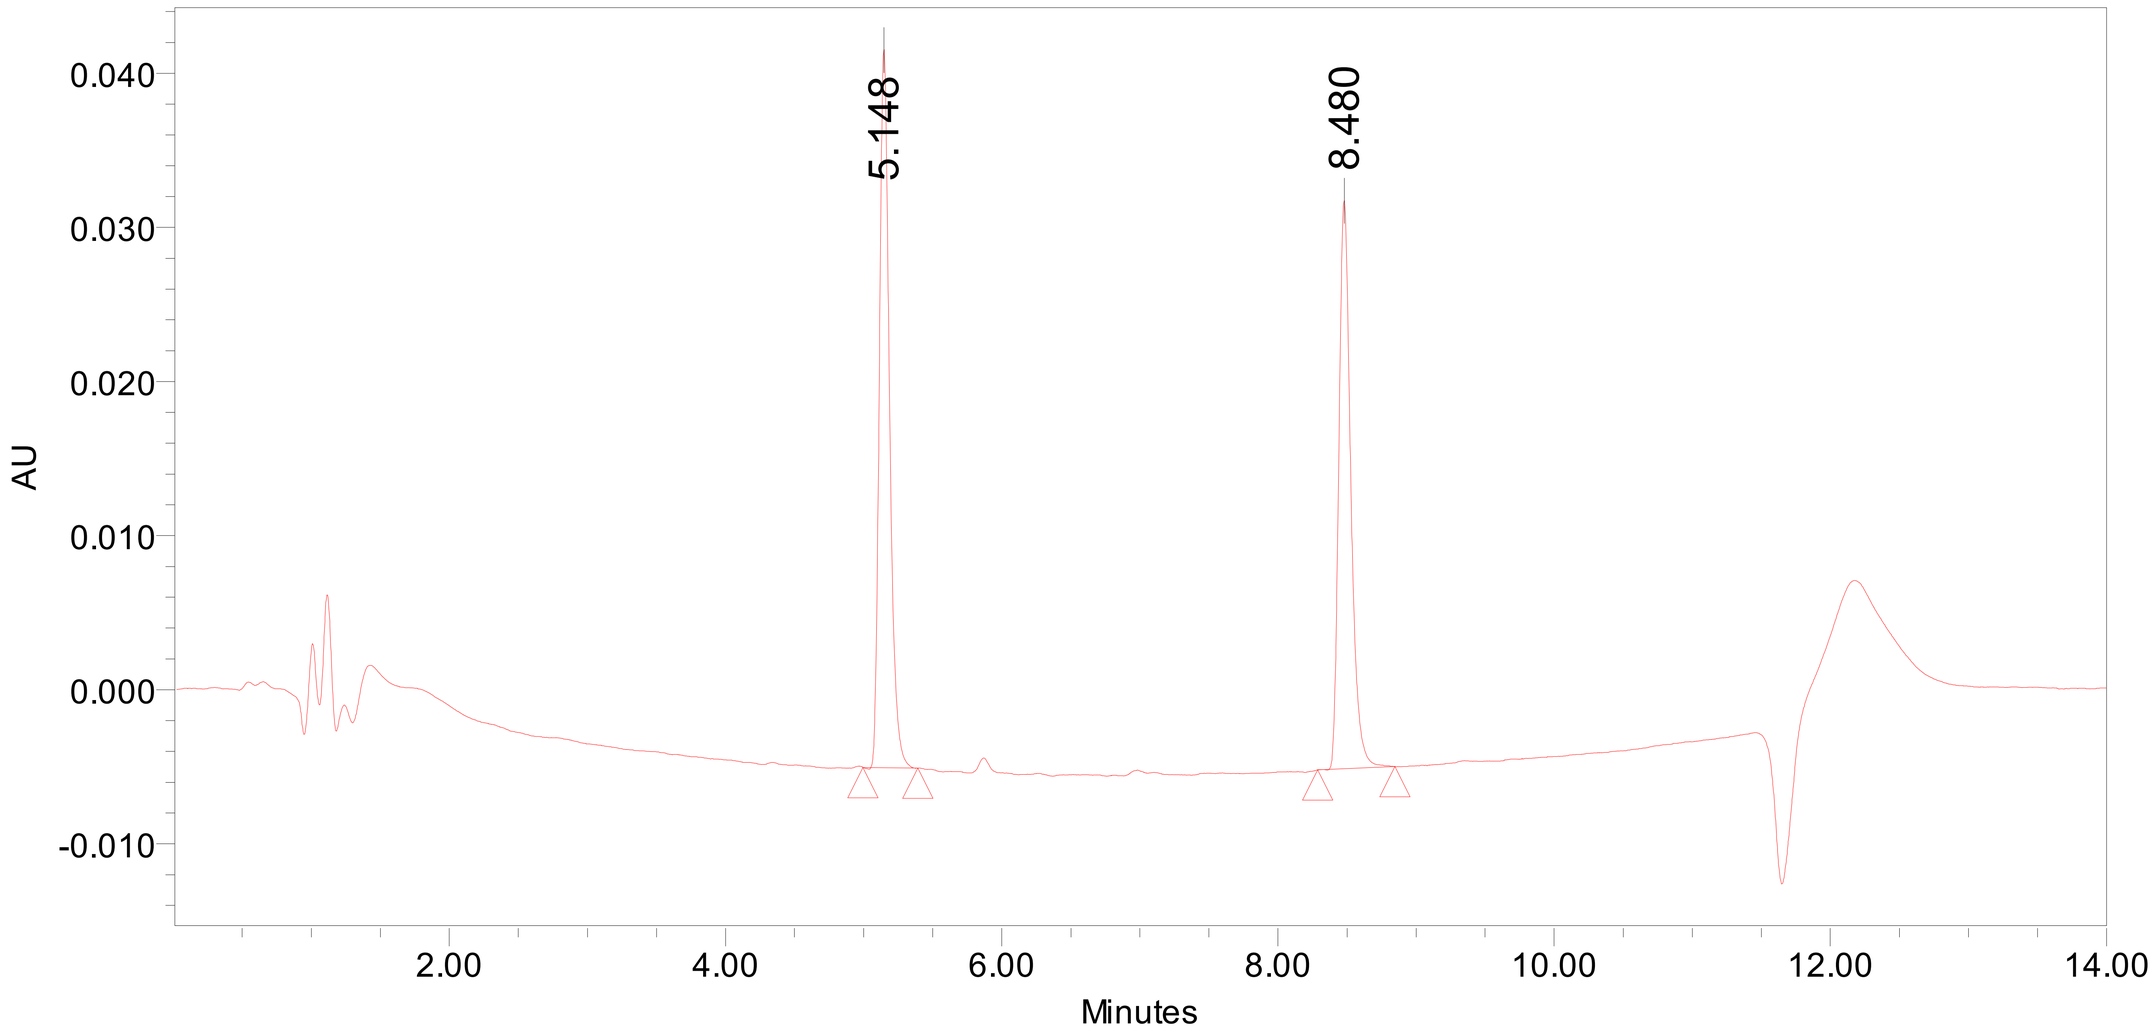

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.148	239398	46609		
2		8.480	222799	36868		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.148					
2		8.480					

SAMPLE INFORMATION

Sample Name:	AV407-Stability-2 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 av407 av422 stab 2ds 3ds
Vial:	71	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-25 15:57:05 CET		
Date Processed:	2025-02-04 14:48:12 CET		

Auto-Scaled Chromatogram

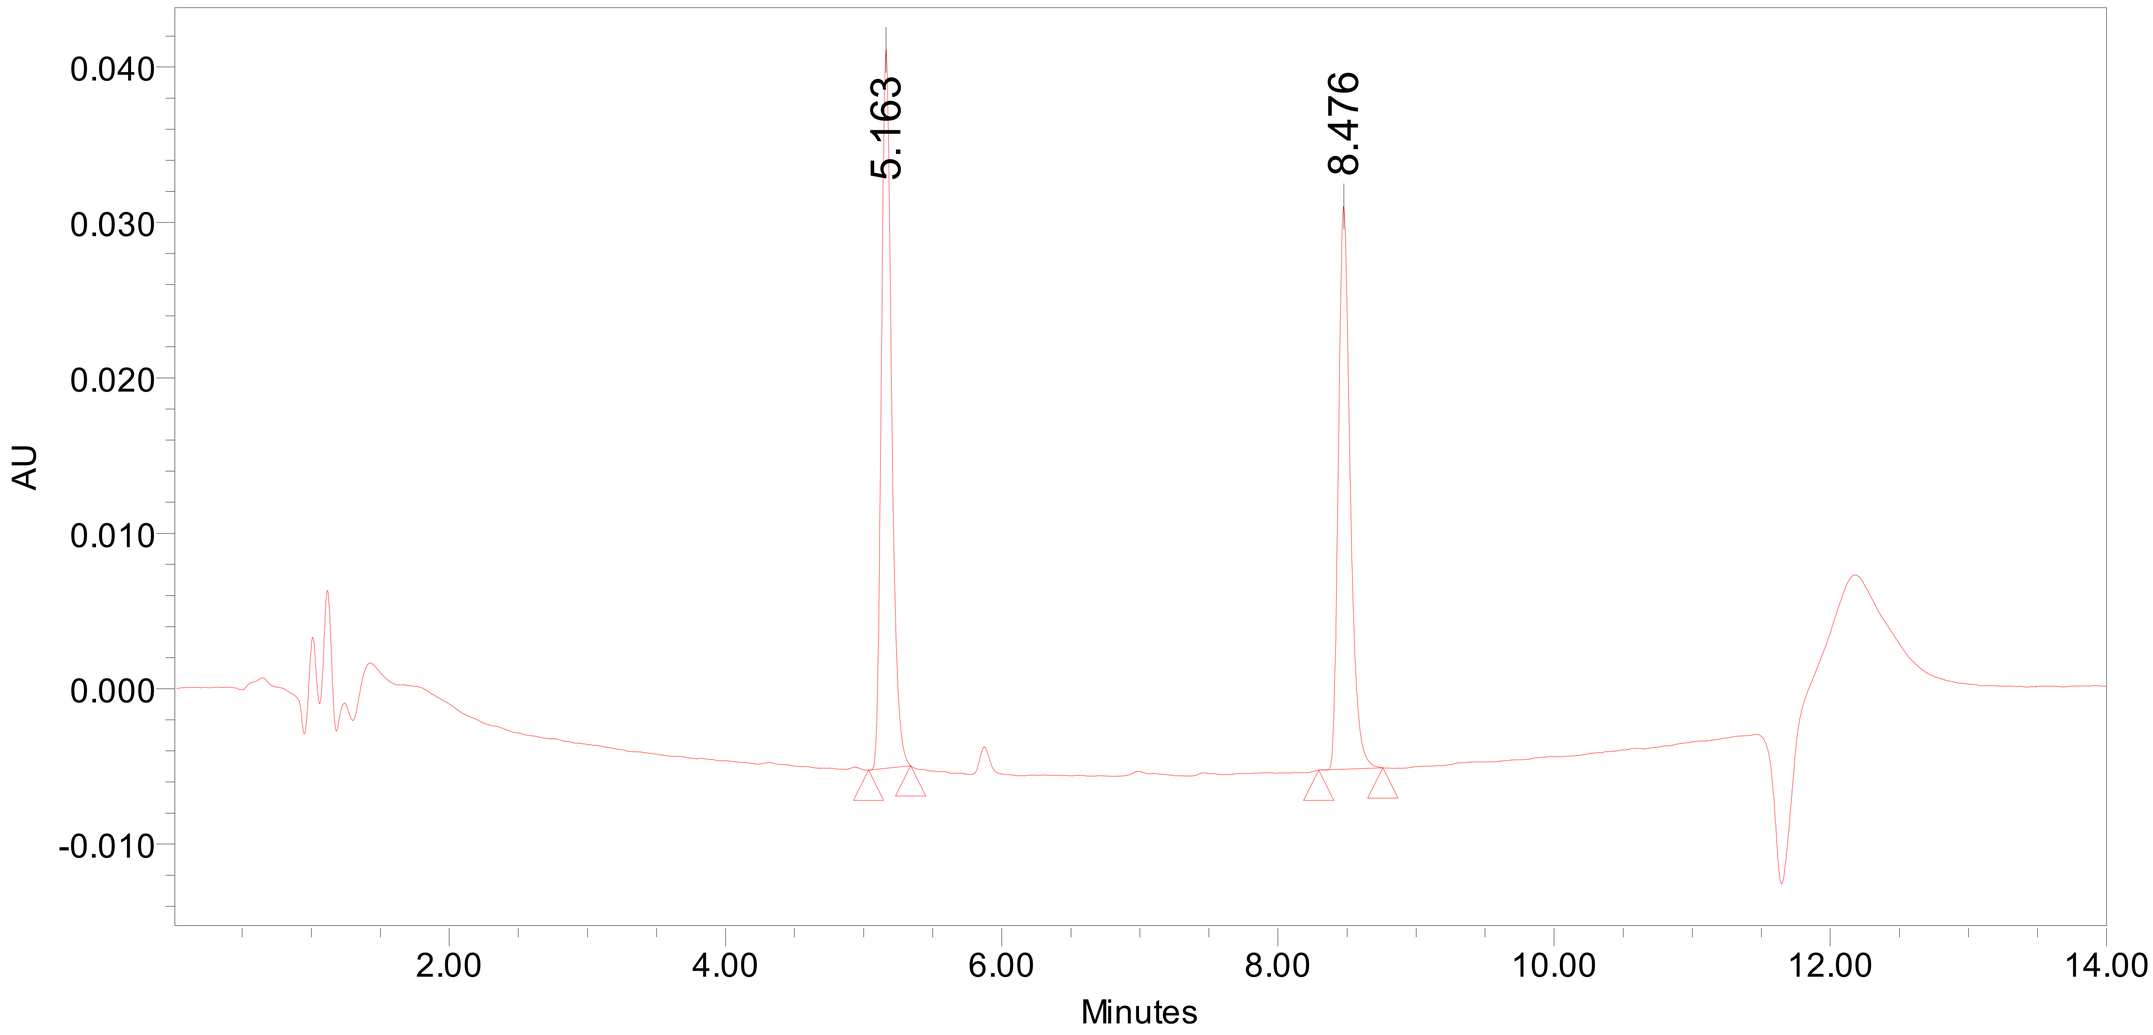

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.163	238134	46249		
2		8.476	216826	36229		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.163					
2		8.476					

SAMPLE INFORMATION

Sample Name:	AV407-Stability-3 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 av407 av422 stab 2ds 3ds
Vial:	71	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-26 14:27:52 CET		
Date Processed:	2025-02-04 14:55:41 CET		

Auto-Scaled Chromatogram

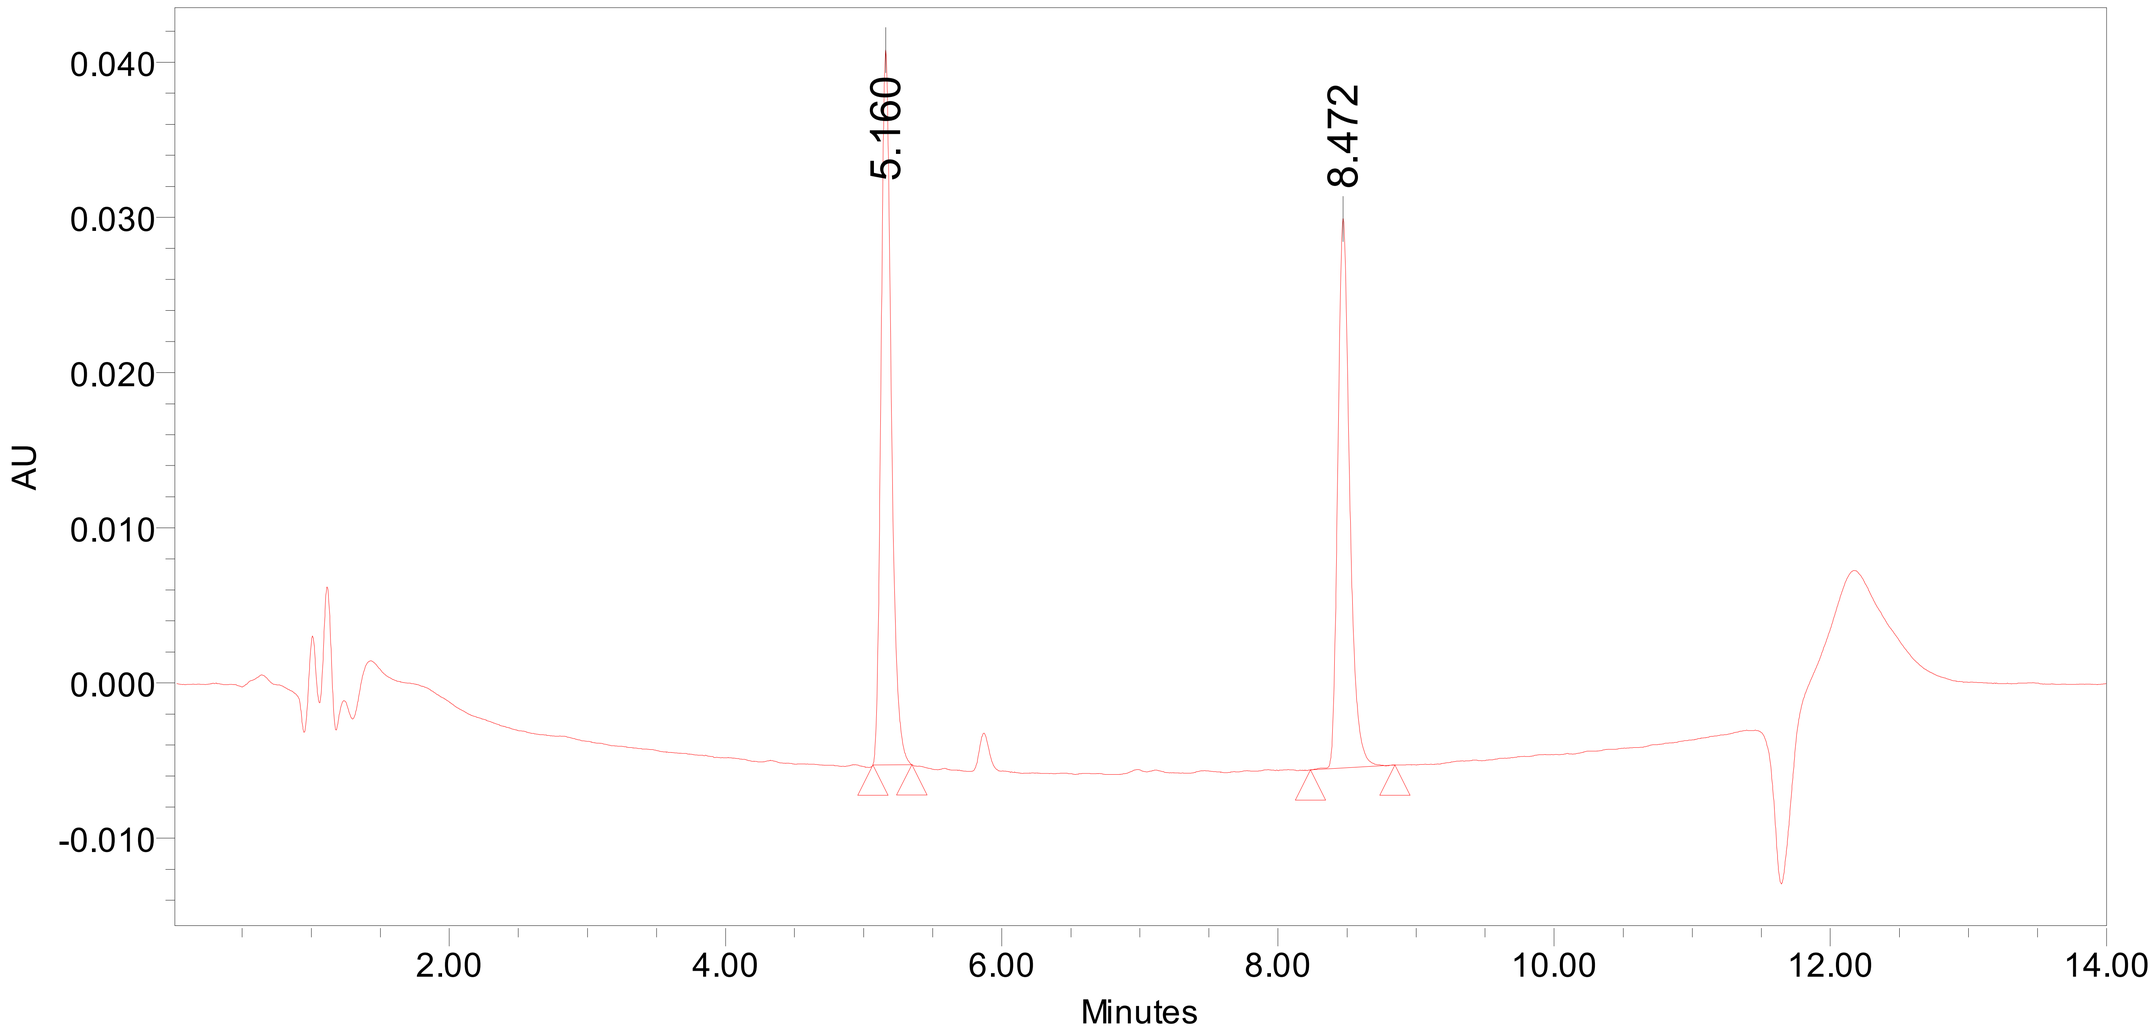

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.160	237209	46102		
2		8.472	212792	35418		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.160					
2		8.472					

SAMPLE INFORMATION

Sample Name:	AV407-Stability-6 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 av407 av422 stab 6d
Vial:	71	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-29 18:17:19 CET		
Date Processed:	2025-02-04 14:48:30 CET		

Auto-Scaled Chromatogram

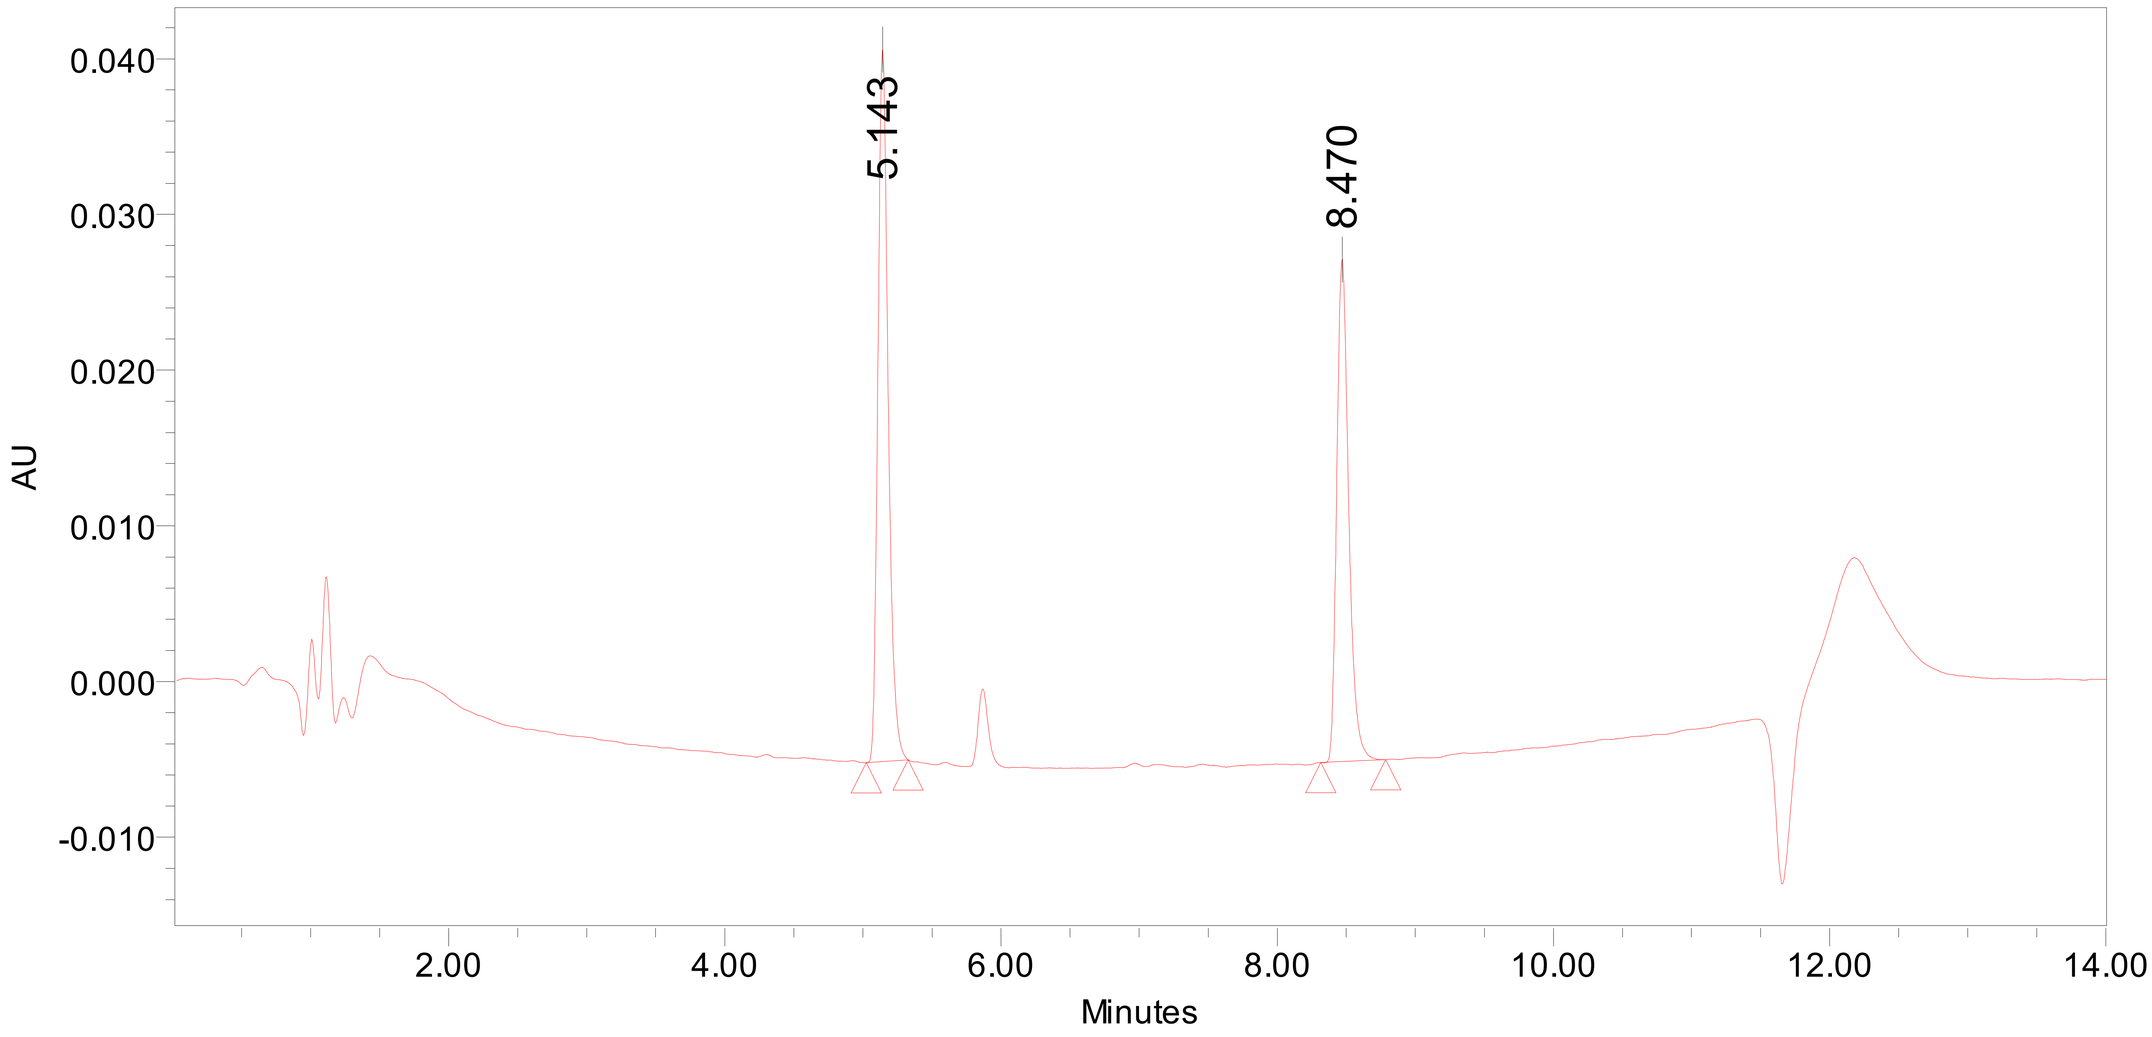

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.143	237702	45741		
2		8.470	194468	32253		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.143					
2		8.470					

SAMPLE INFORMATION

Sample Name:	AV407-Stability-7 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	AV320SO AV407 AV422 STAB 7d
Vial:	71	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-30 16:38:18 CET		
Date Processed:	2025-02-04 14:48:53 CET		

Auto-Scaled Chromatogram

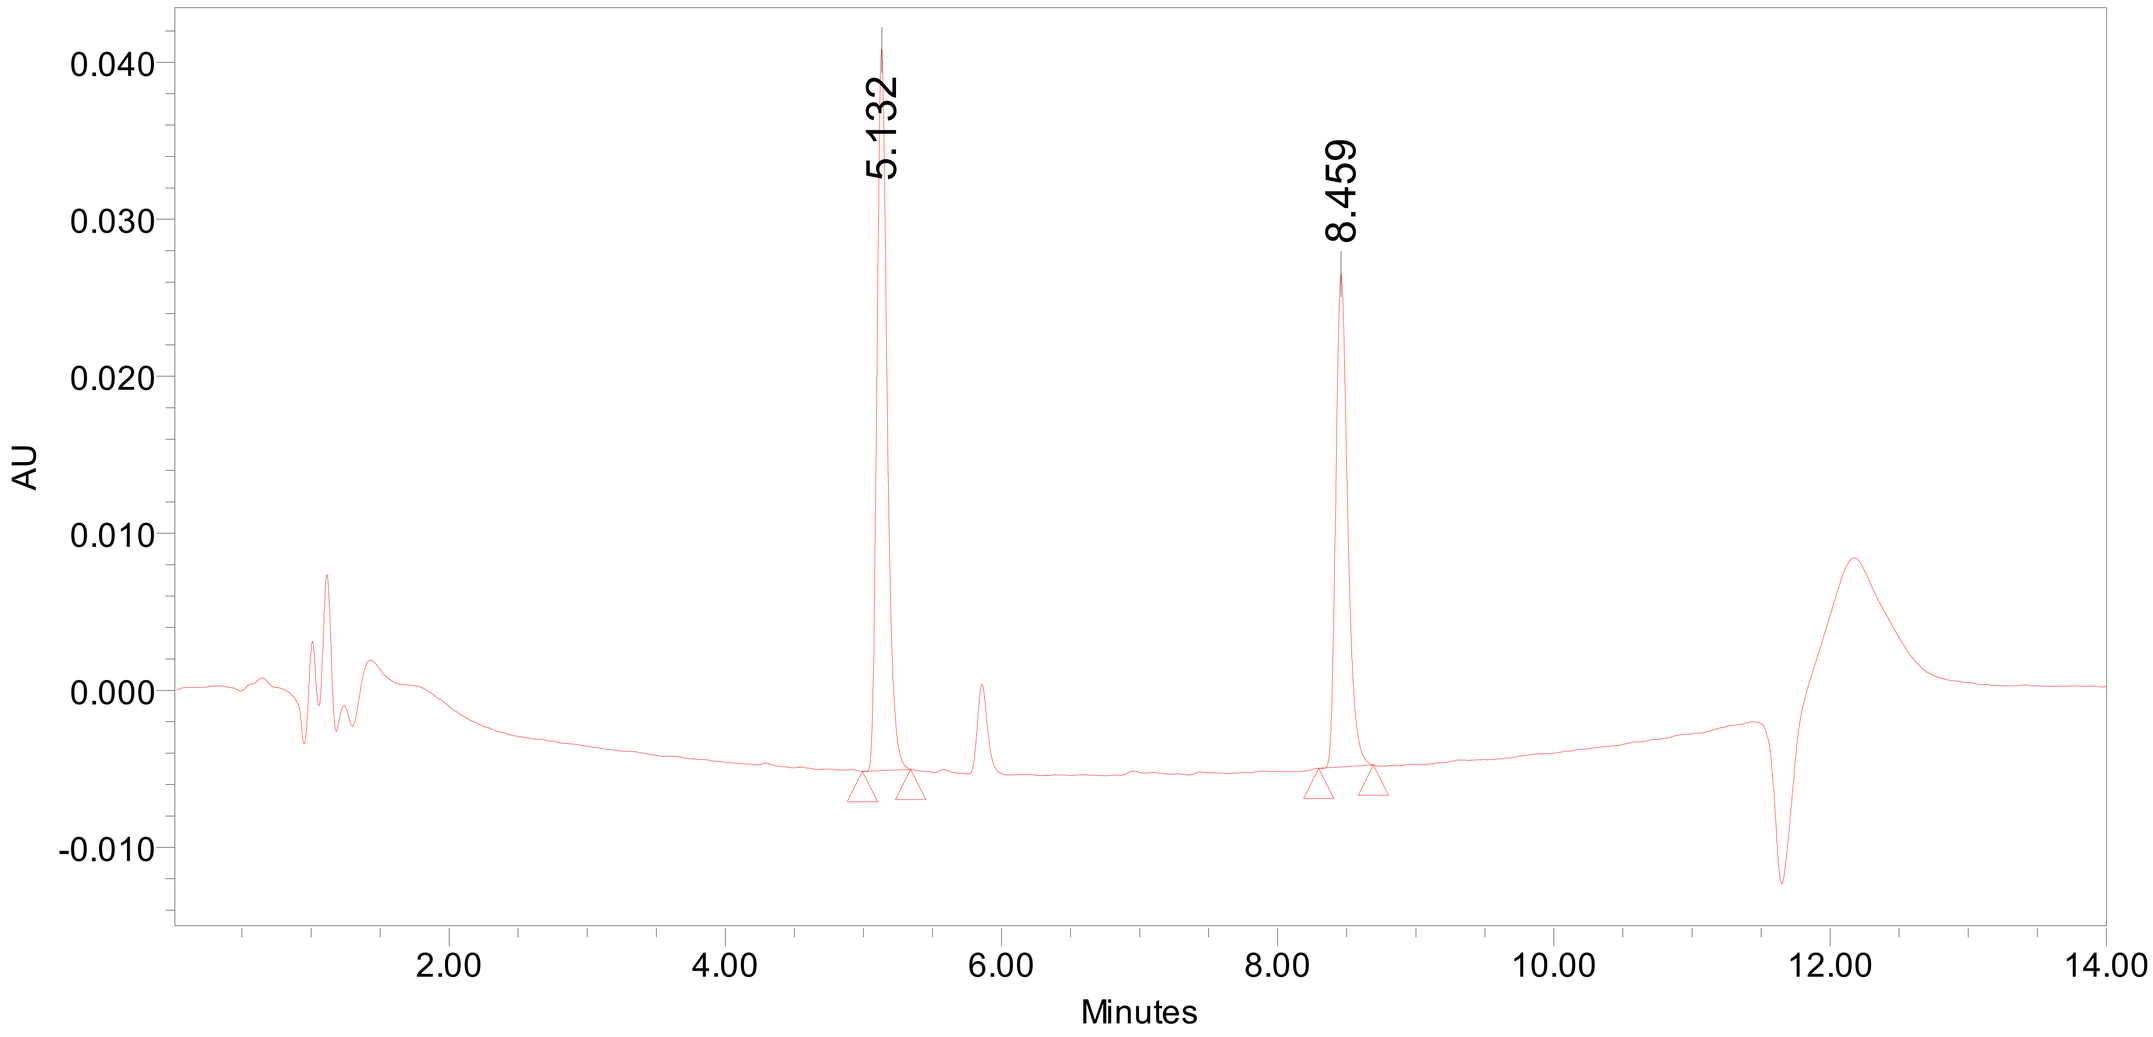

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.132	238101	45920		
2		8.459	188565	31418		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.132					
2		8.459					