
Untitled

SAMPLE INFORMATION

Sample Name:	AV400-SO-0	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	STABILITY 0
Vial:	36	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-08 03:05:36 CET		
Date Processed:	2025-01-20 14:18:50 CET		

Auto-Scaled Chromatogram

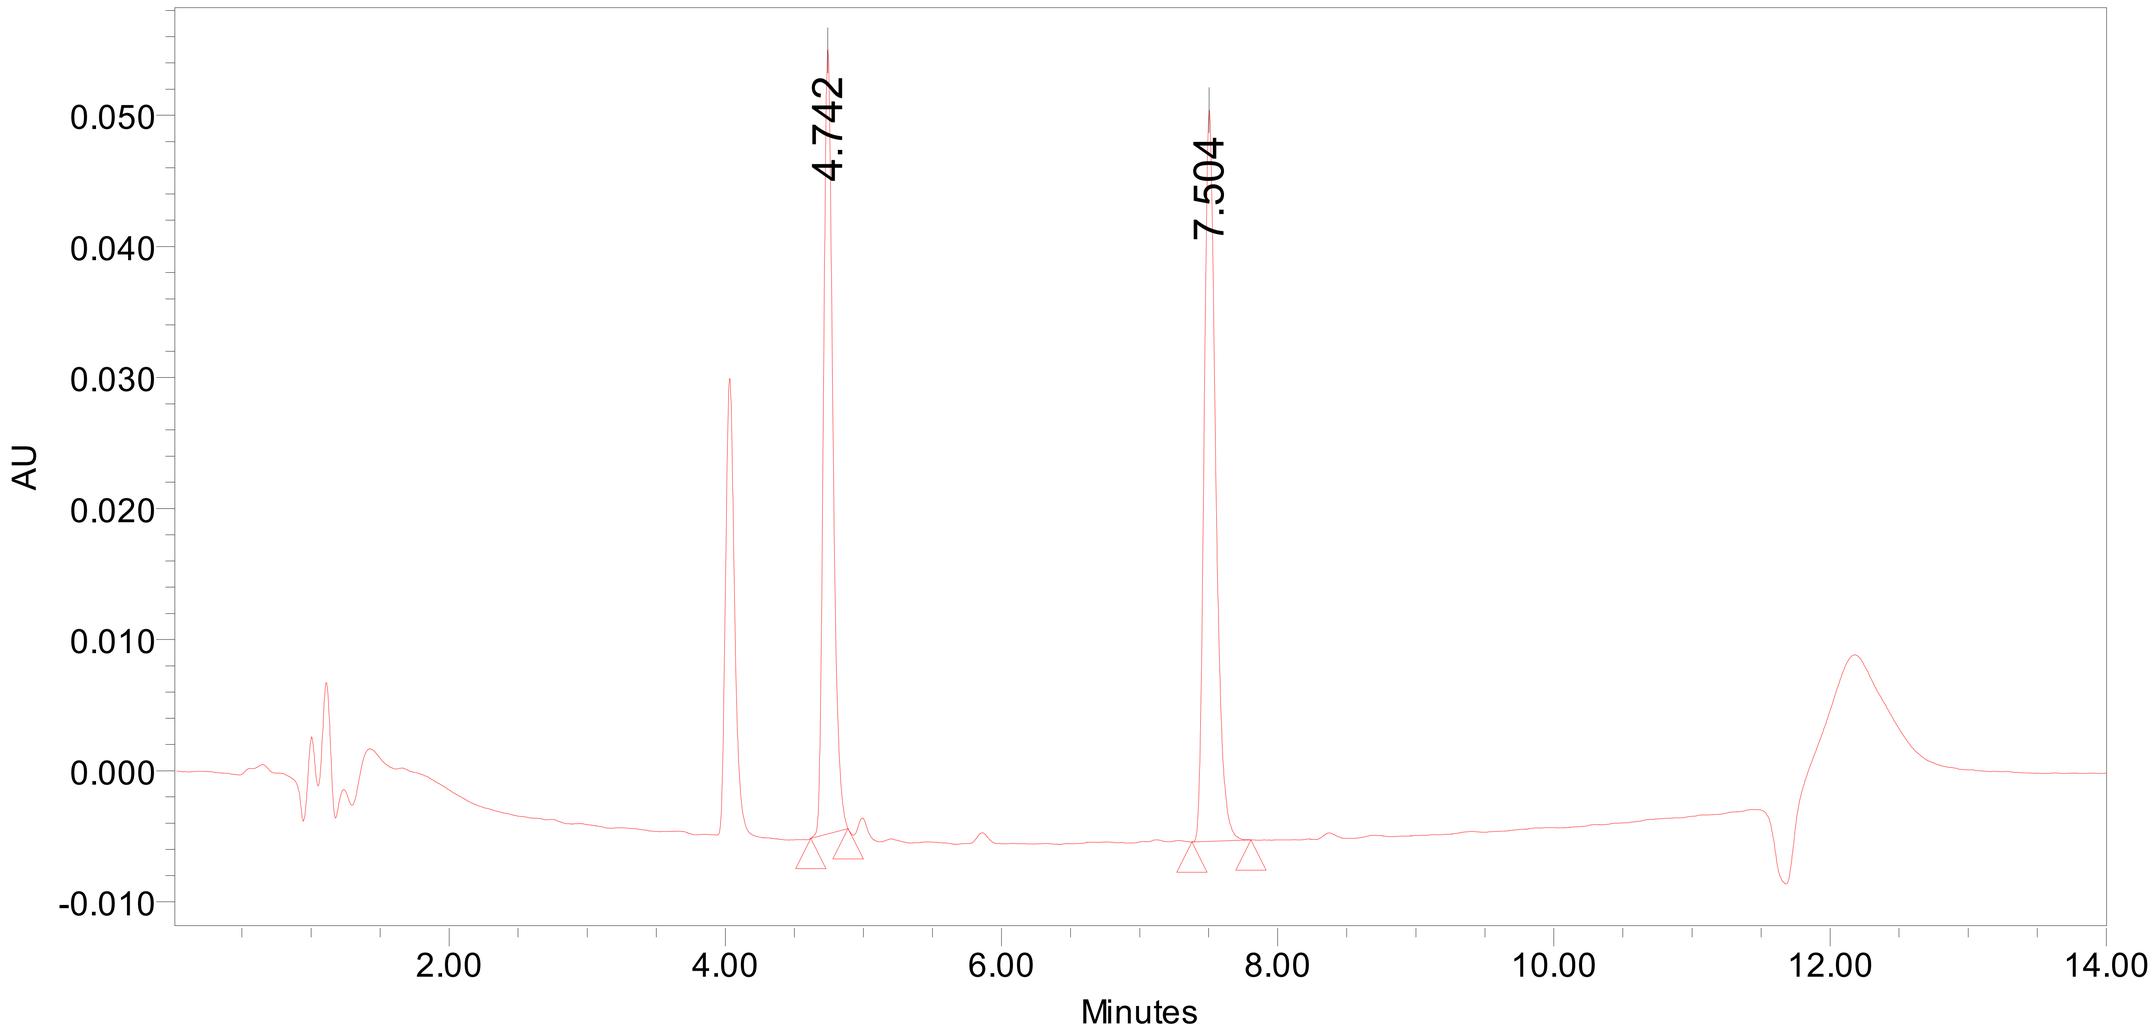

Peak Results

	Name	RT	Area	Height	Amount	Units
1		4.742	284643	59857		
2		7.504	327051	55805		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		4.742					
2		7.504					

SAMPLE INFORMATION

Sample Name:	AV400-SO-Stability 1 day	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability 1 day
Vial:	36	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-09 00:21:19 CET		
Date Processed:	2025-01-20 14:19:12 CET		

Auto-Scaled Chromatogram

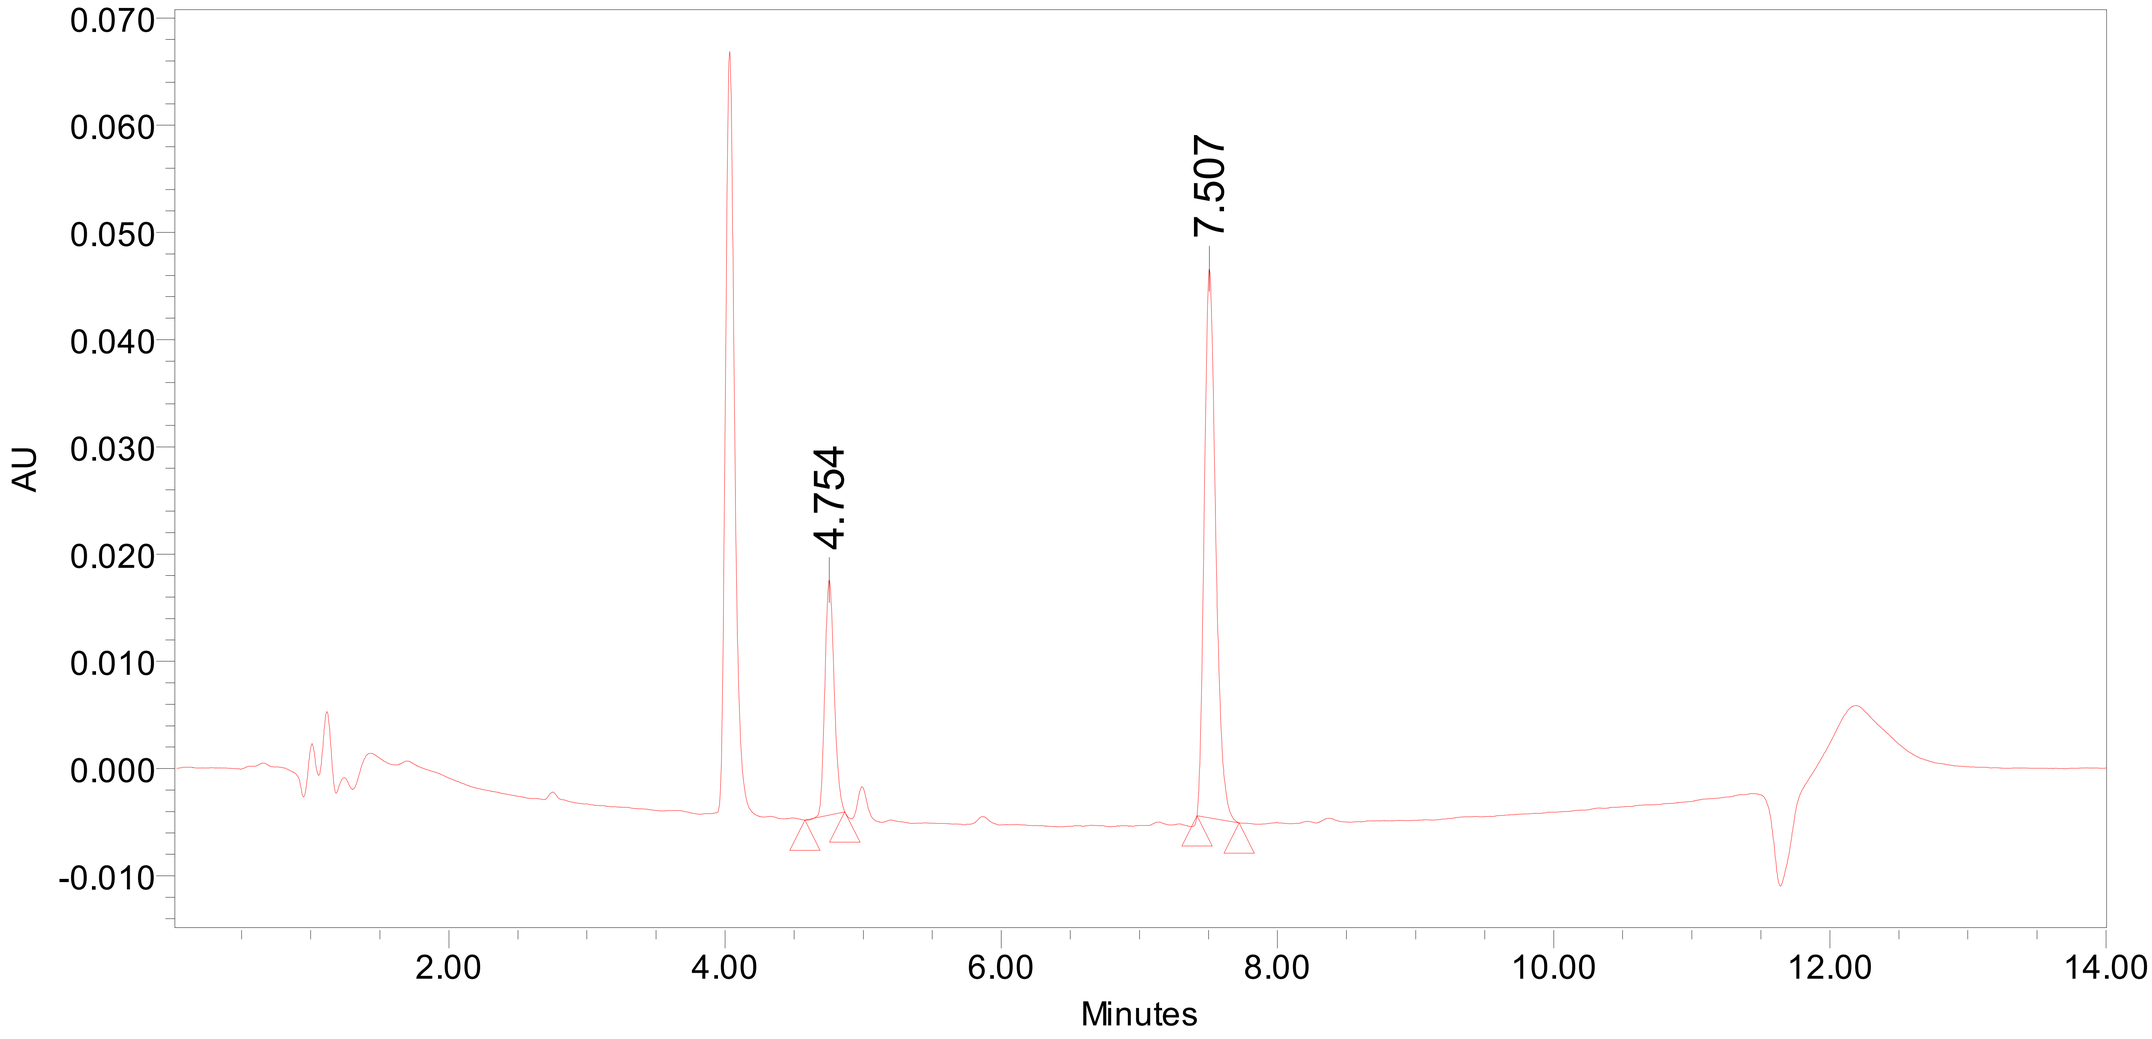

Peak Results

	Name	RT	Area	Height	Amount	Units
1		4.754	102983	21930		
2		7.507	295557	51211		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		4.754					
2		7.507					

SAMPLE INFORMATION

Sample Name:	AV400-SO-Stability 2 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability 2 days
Vial:	36	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-10 00:32:16 CET		
Date Processed:	2025-01-20 14:19:43 CET		

Auto-Scaled Chromatogram

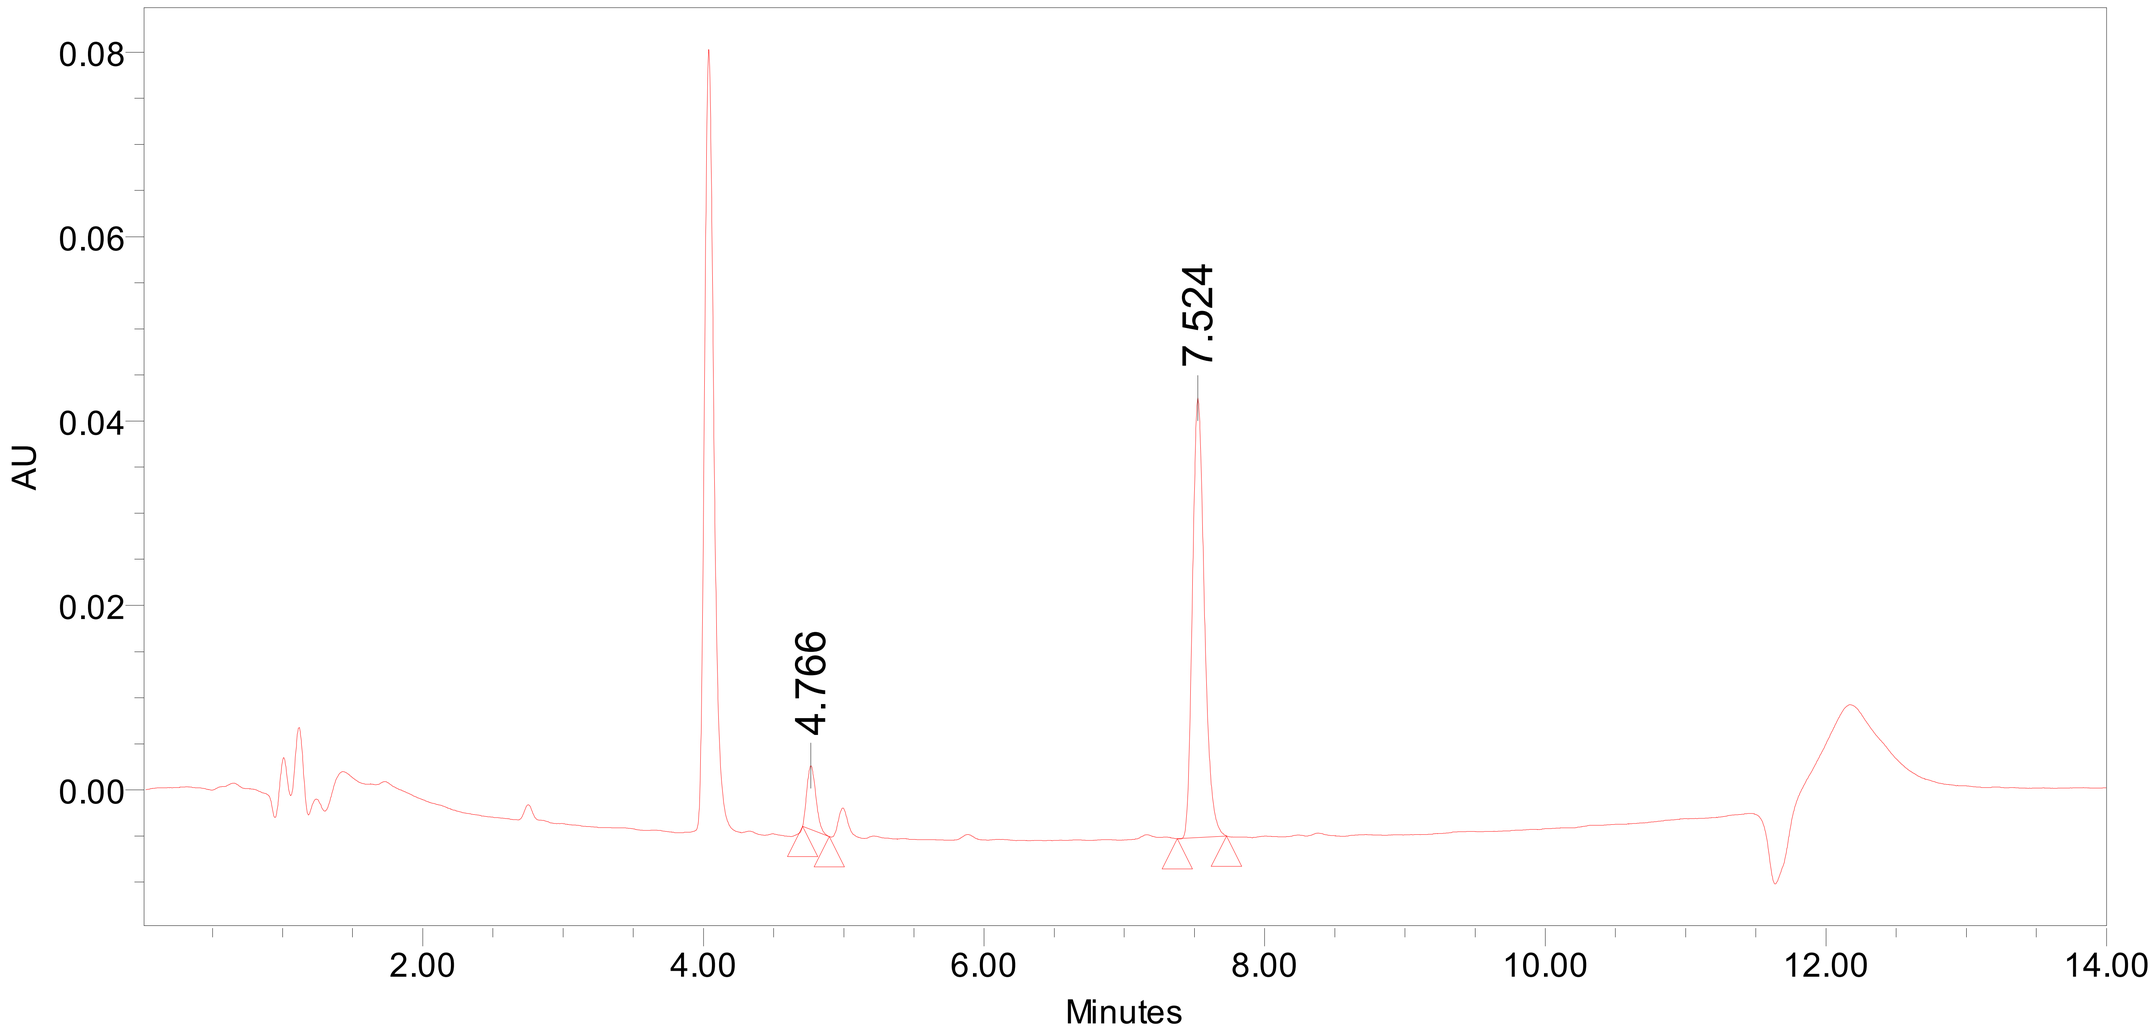

Peak Results

	Name	RT	Area	Height	Amount	Units
1		4.766	30581	6934		
2		7.524	280779	47665		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		4.766					
2		7.524					

SAMPLE INFORMATION

Sample Name:	AV400-SO-Stability 3 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 3 days
Vial:	36	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-11 00:08:09 CET		
Date Processed:	2025-01-20 14:20:02 CET		

Auto-Scaled Chromatogram

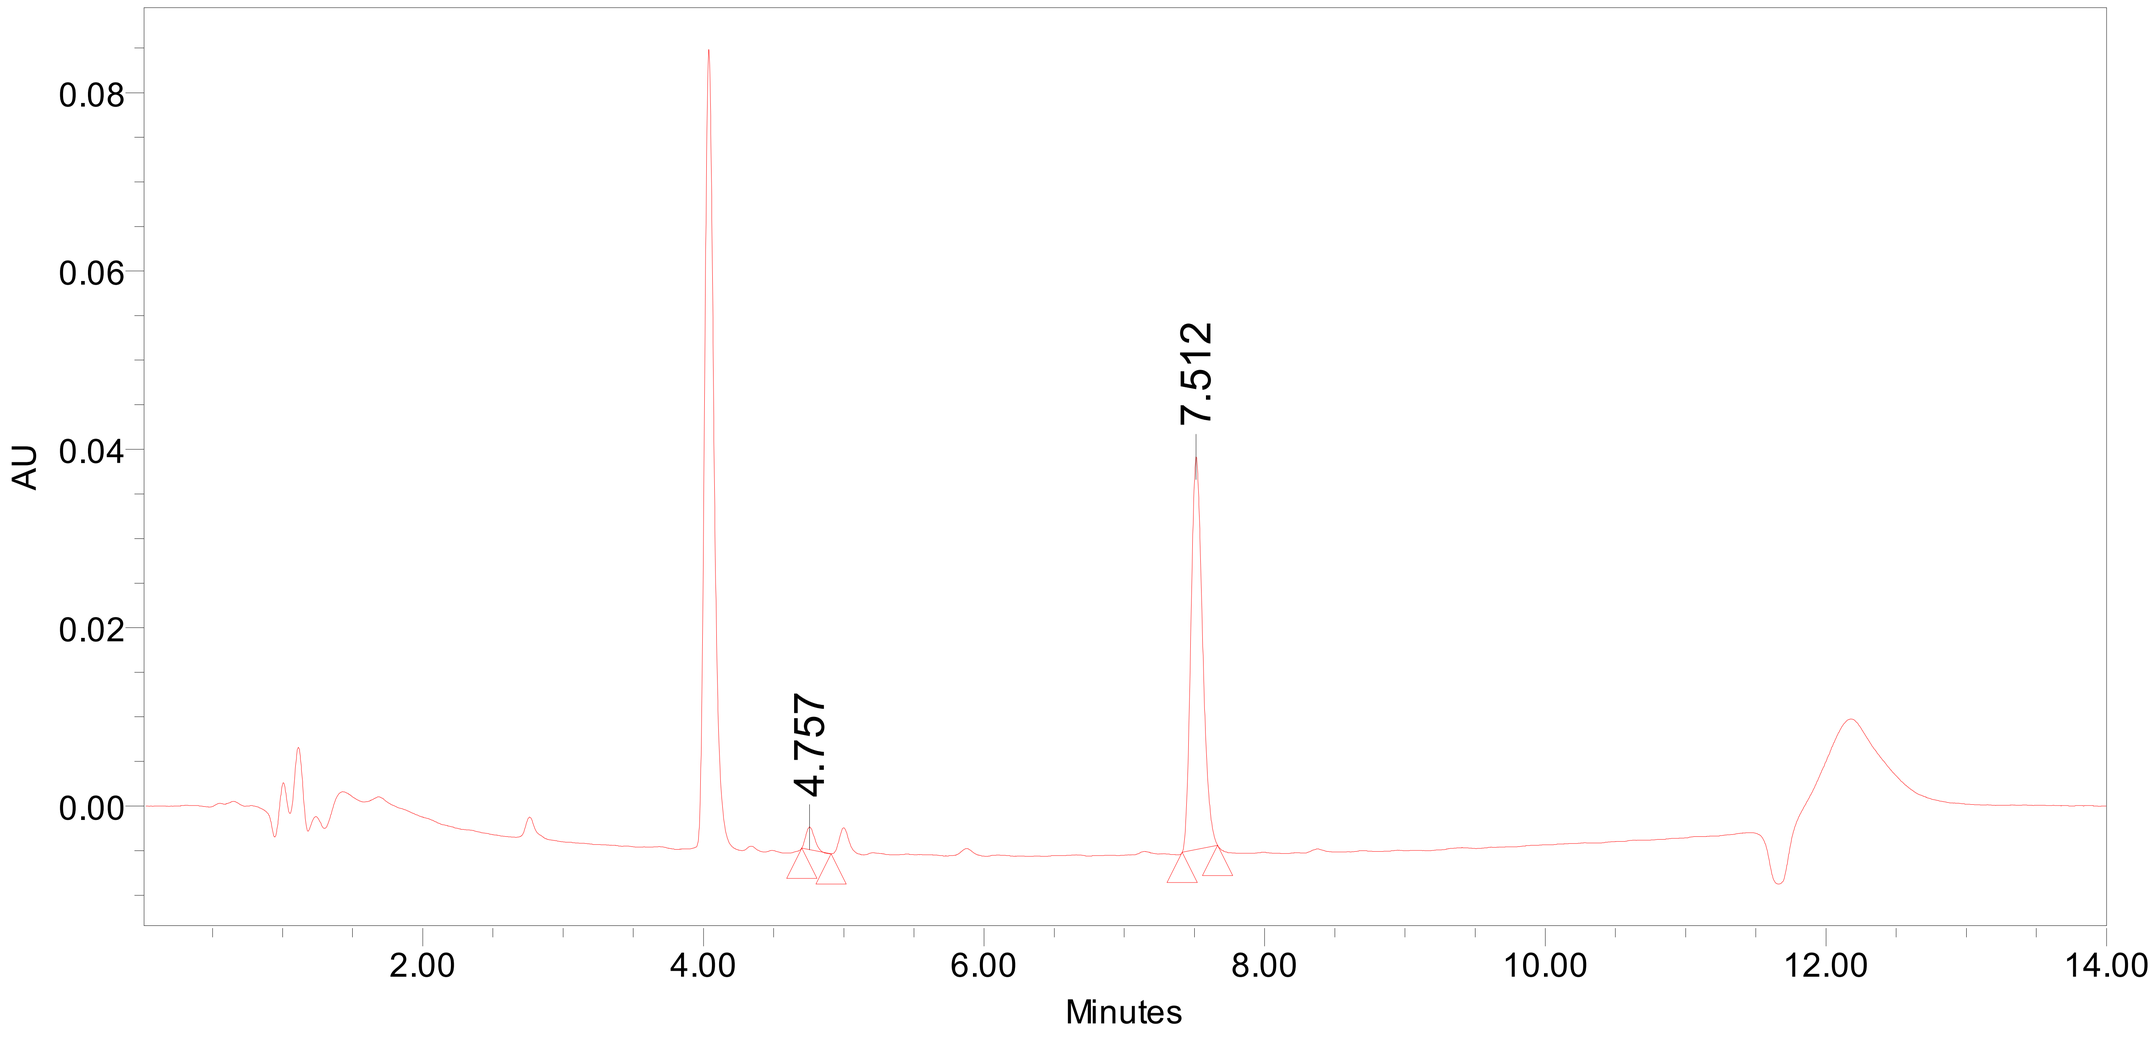

Peak Results

	Name	RT	Area	Height	Amount	Units
1		4.757	10732	2520		
2		7.512	252719	44054		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		4.757					
2		7.512					

SAMPLE INFORMATION

Sample Name:	AV400-SO-Stability 4 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 4 days
Vial:	36	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-11 20:52:08 CET		
Date Processed:	2025-01-20 14:20:23 CET		

Auto-Scaled Chromatogram

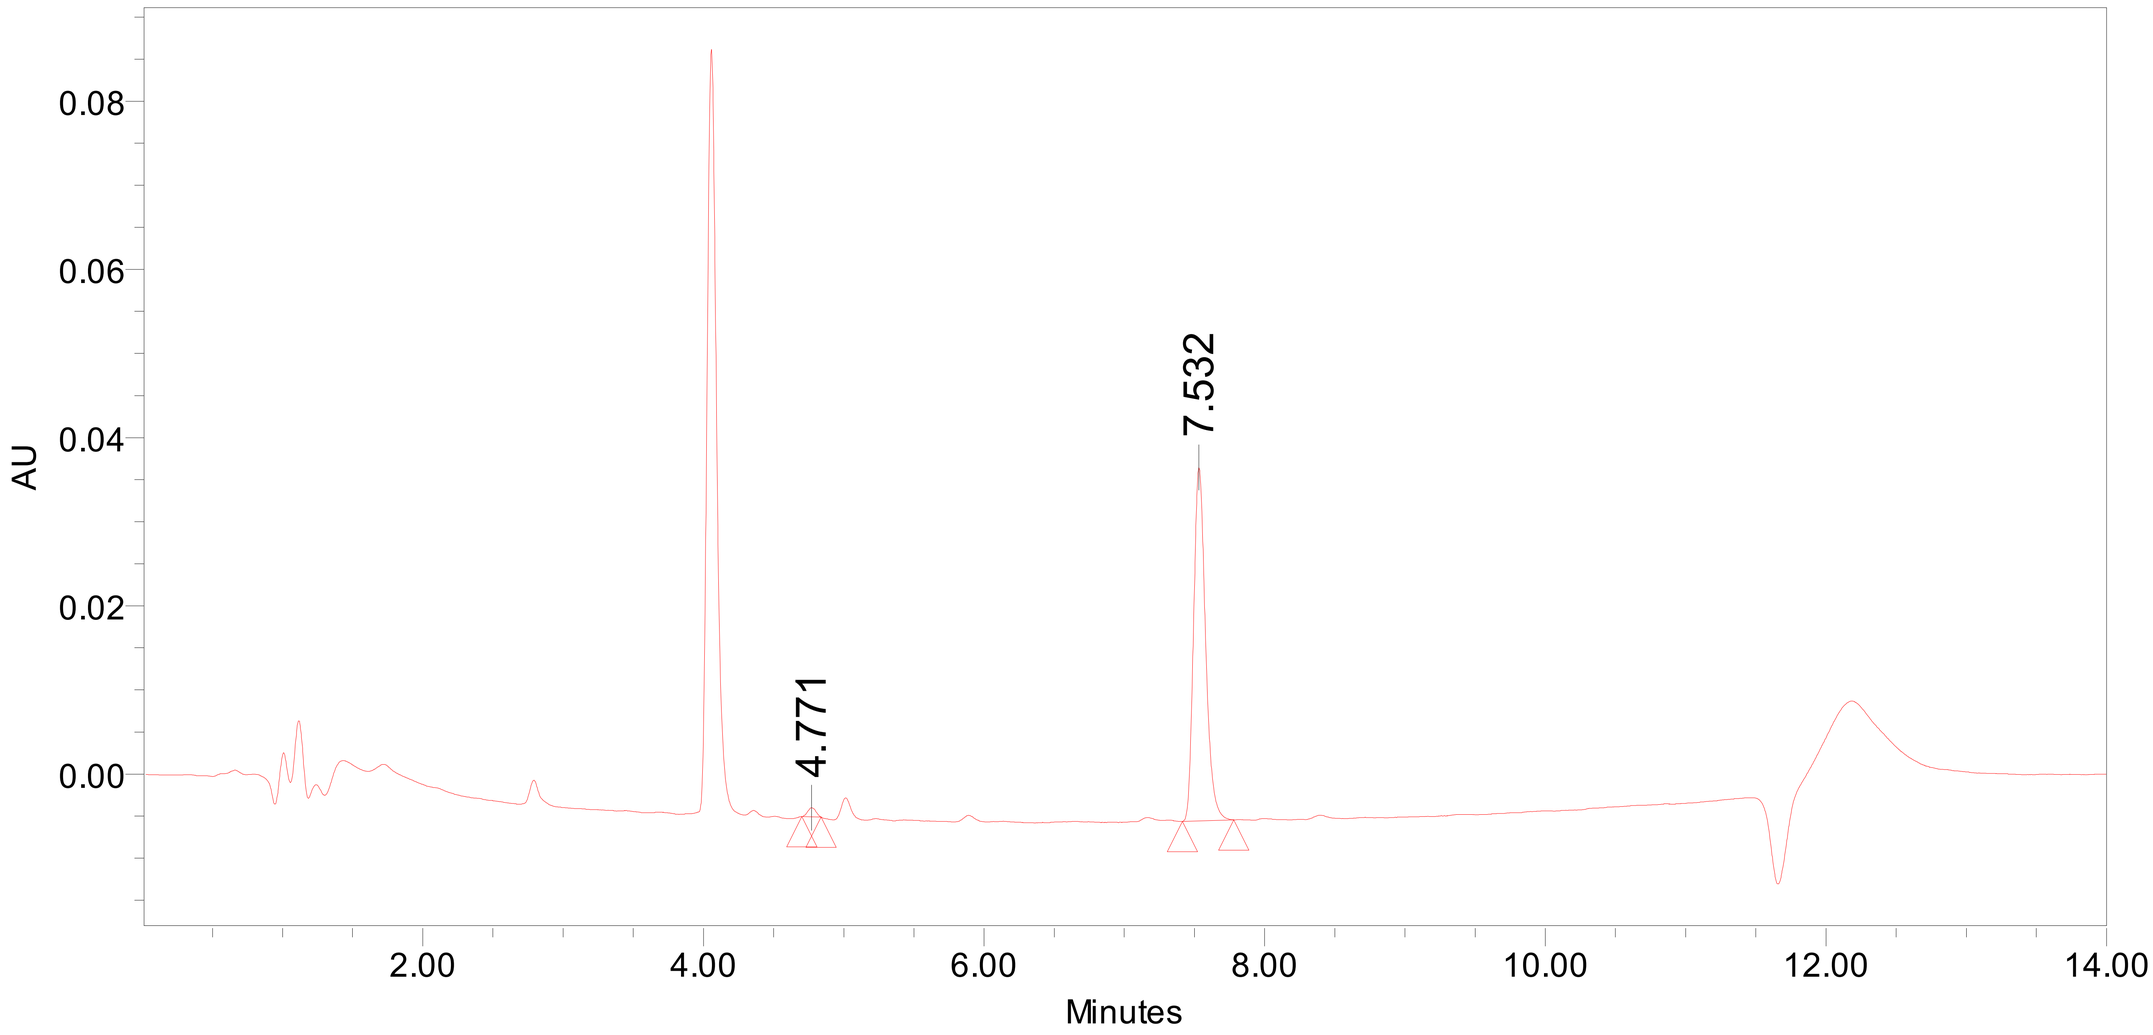

Peak Results

	Name	RT	Area	Height	Amount	Units
1		4.771	4461	1099		
2		7.532	248207	42043		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		4.771					
2		7.532					

SAMPLE INFORMATION

Sample Name:	AV400-SO-Stability 6 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability 6 days
Vial:	36	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-13 19:09:15 CET		
Date Processed:	2025-01-20 14:21:02 CET		

Auto-Scaled Chromatogram

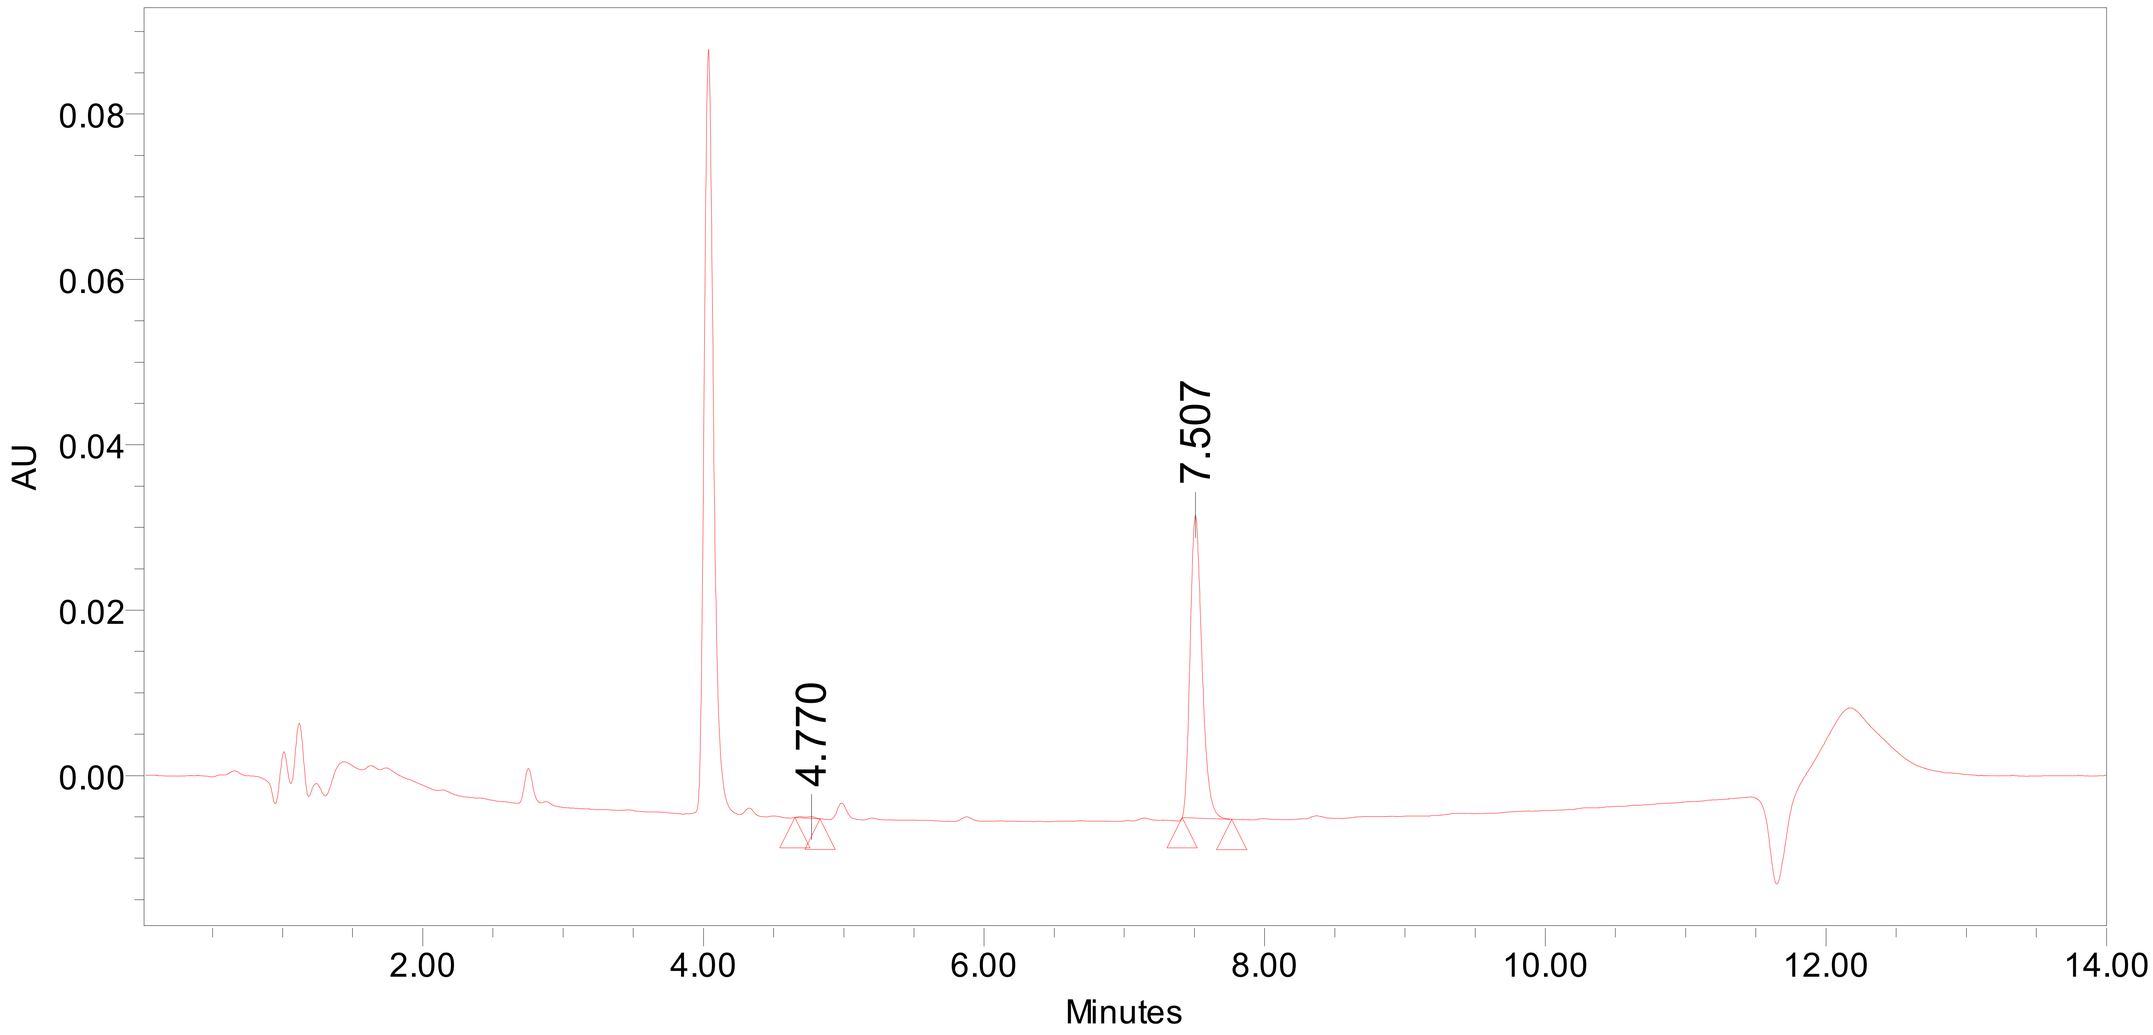

Peak Results

	Name	RT	Area	Height	Amount	Units
1		4.770	1219	191		
2		7.507	213181	36641		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		4.770					
2		7.507					