
SAMPLE INFORMATION

Sample Name:	AV320-SO2-SStability 1 day	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 so2 stab 1 day
Vial:	80	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-05 16:39:56 CET		
Date Processed:	2025-02-05 17:05:56 CET		

Auto-Scaled Chromatogram

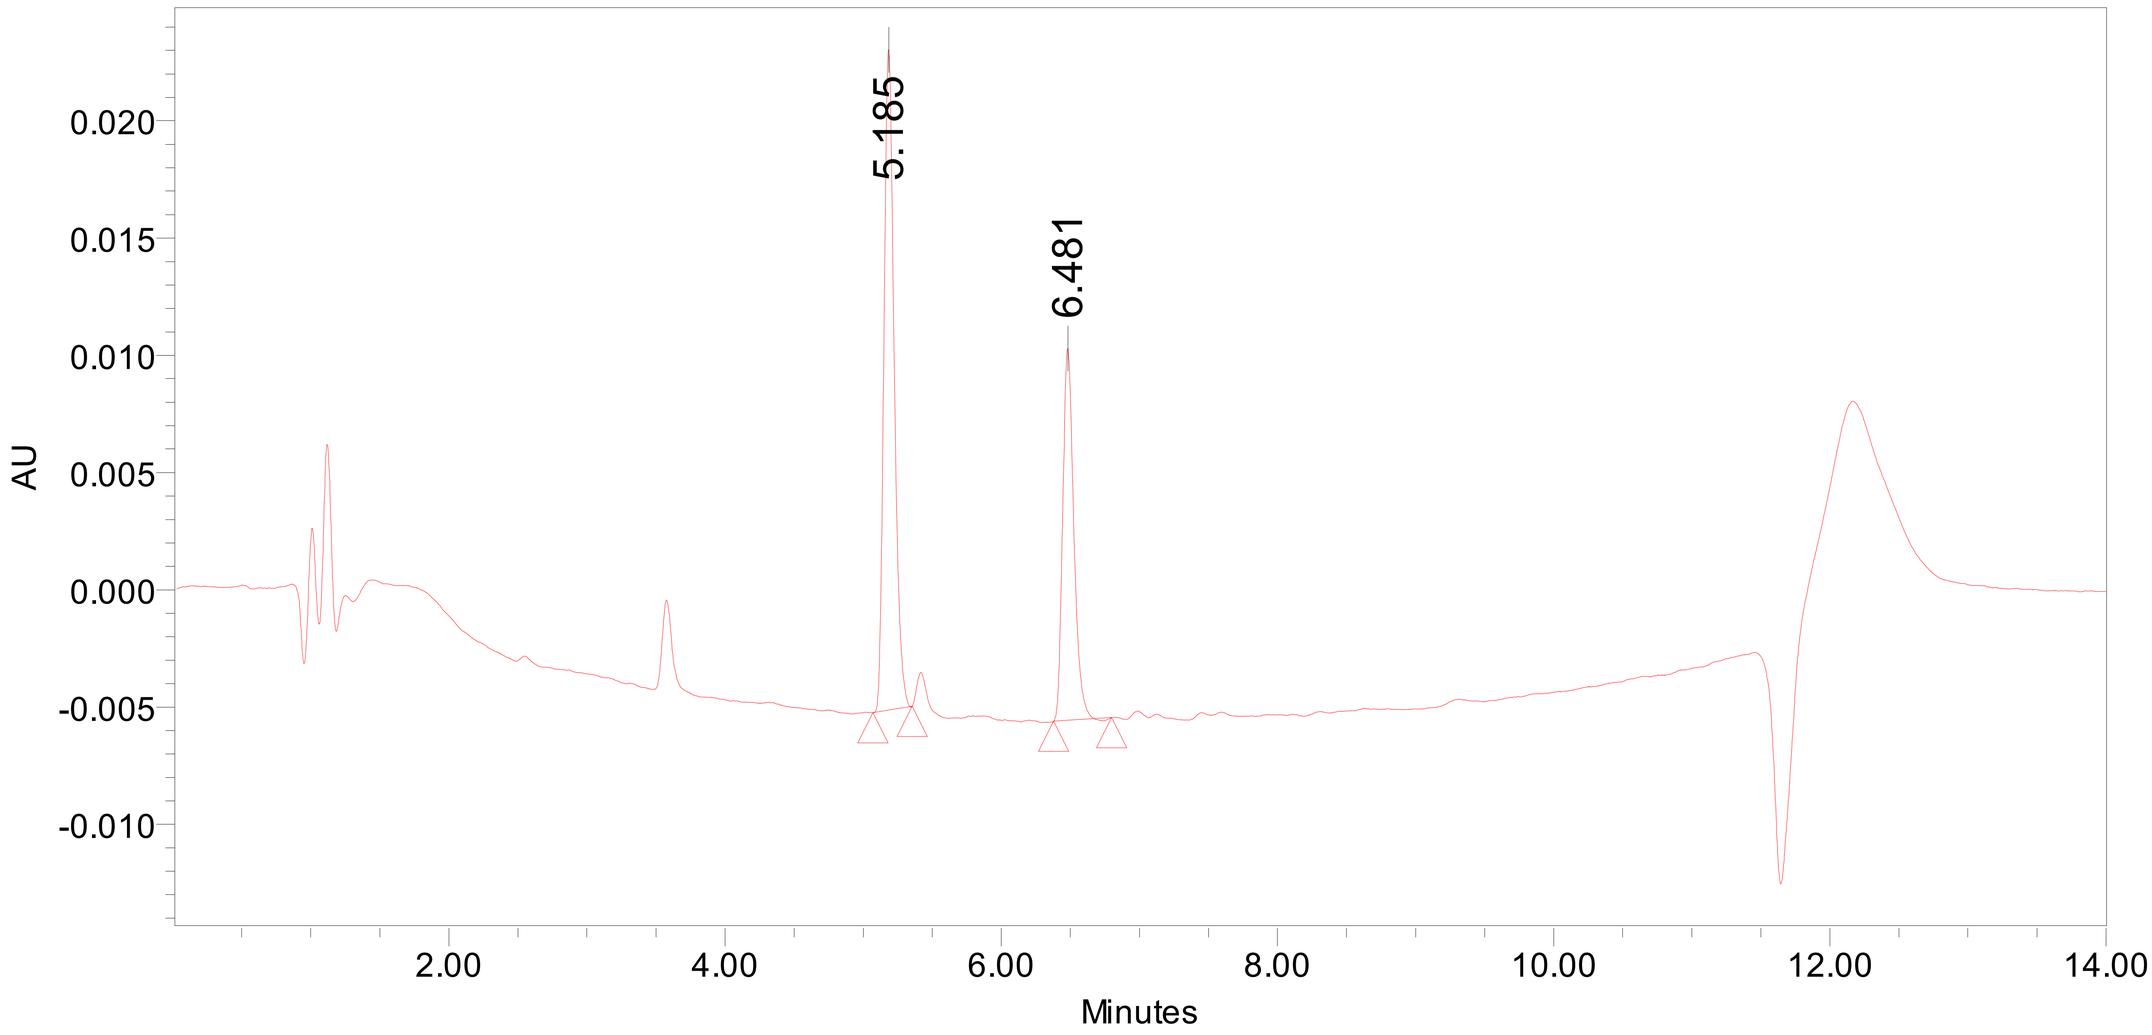

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.185	145252	28173		
2		6.481	89406	15860		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.185					
2		6.481					

SAMPLE INFORMATION

Sample Name:	AV320-SO2-Stability-2 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 so2 stability 2 days
Vial:	80	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-06 16:31:21 CET		
Date Processed:	2025-02-07 11:57:56 CET		

Auto-Scaled Chromatogram

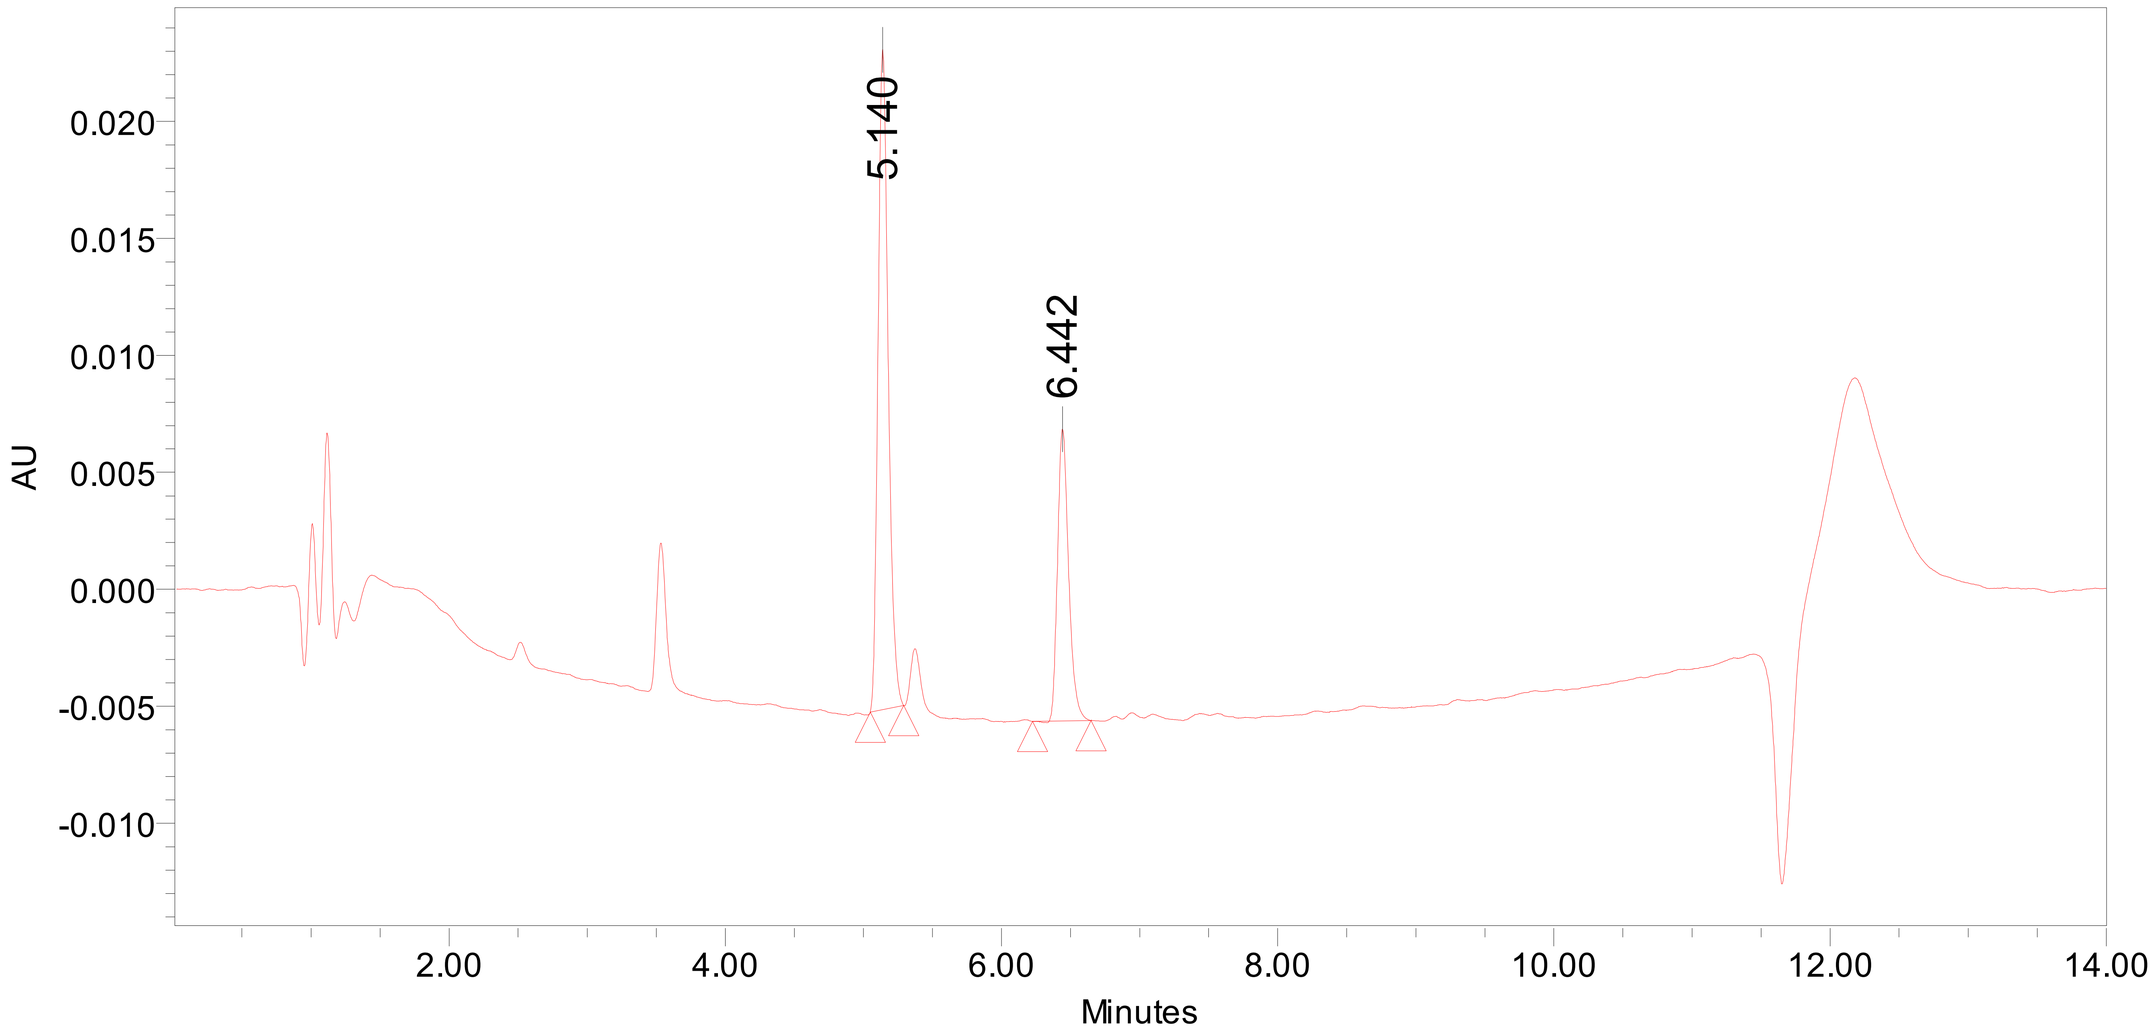

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.140	144936	28201		
2		6.442	70166	12478		

PDA Result Table


	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.140					
2		6.442					

Untitled

SAMPLE INFORMATION

Sample Name:	AV320-SO2-Stability-4 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	av320 so2 stability 4 days
Vial:	80	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-02-08 02:41:22 CET		
Date Processed:	2025-02-10 10:22:29 CET		

Auto-Scaled Chromatogram

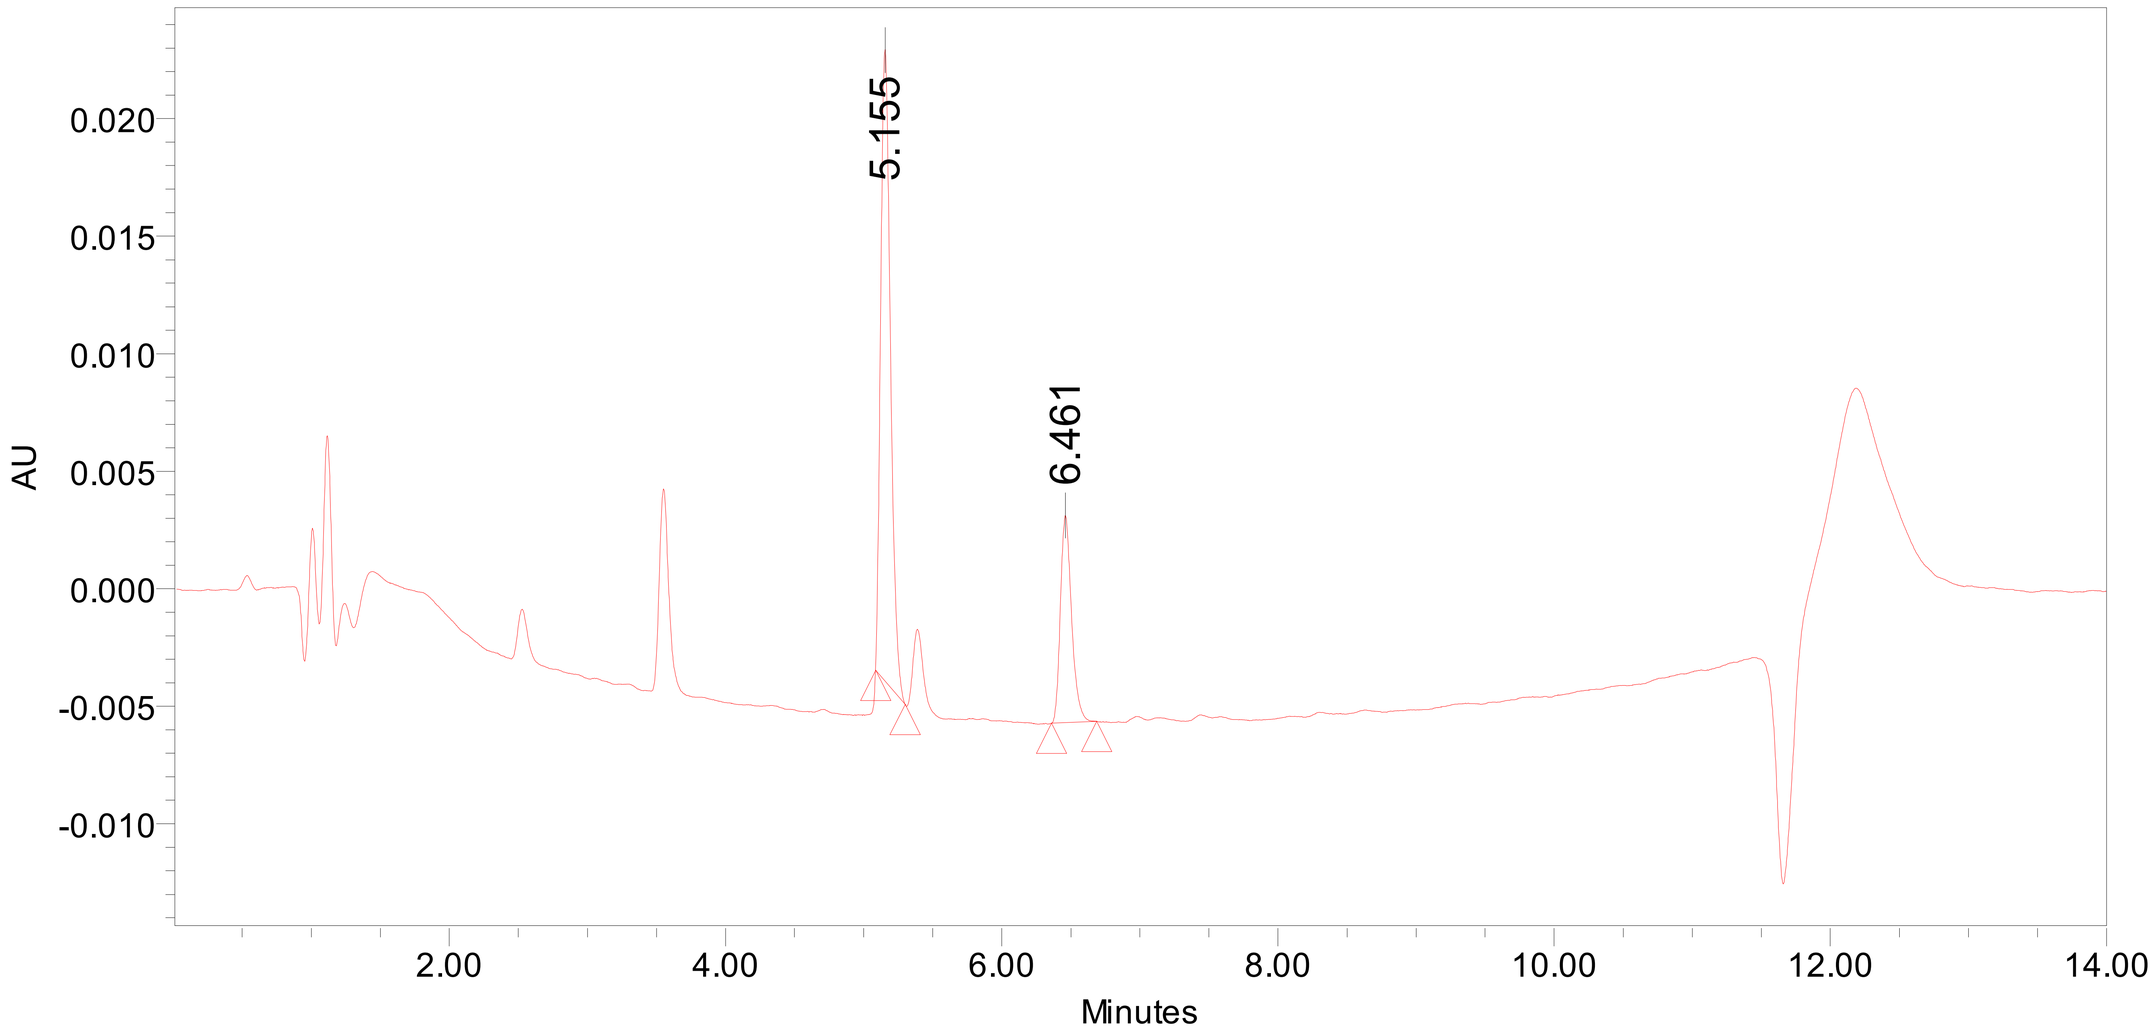

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.155	133367	26880		
2		6.461	49710	8824		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.155					
2		6.461					