
SAMPLE INFORMATION

Sample Name:	HK21_Stability again_0	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-05 17:31:37 CET		
Date Processed:	2025-03-12 09:52:52 CET		

Auto-Scaled Chromatogram

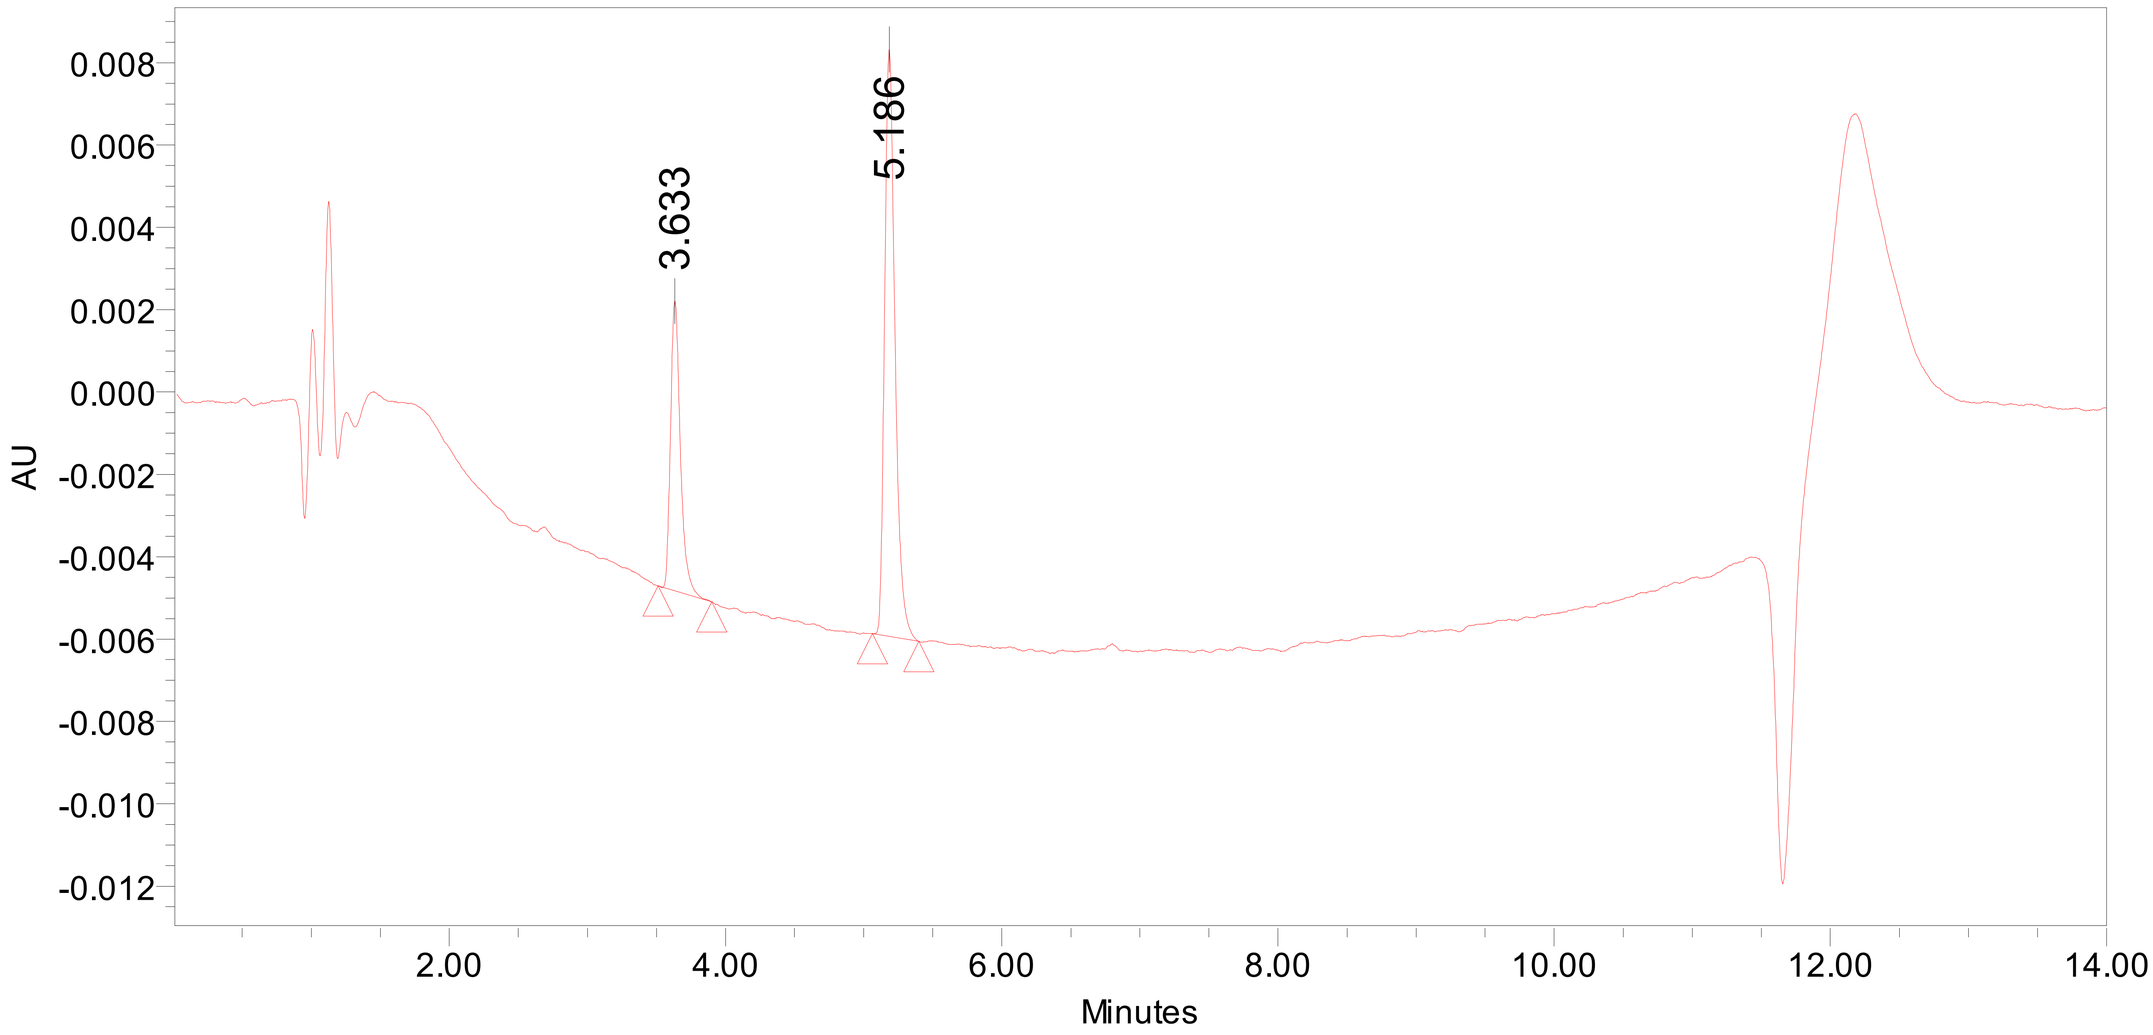

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.633	35005	7043		
2		5.186	74544	14255		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.633					
2		5.186					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_1 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-05 18:50:12 CET		
Date Processed:	2025-03-12 09:53:12 CET		

Auto-Scaled Chromatogram

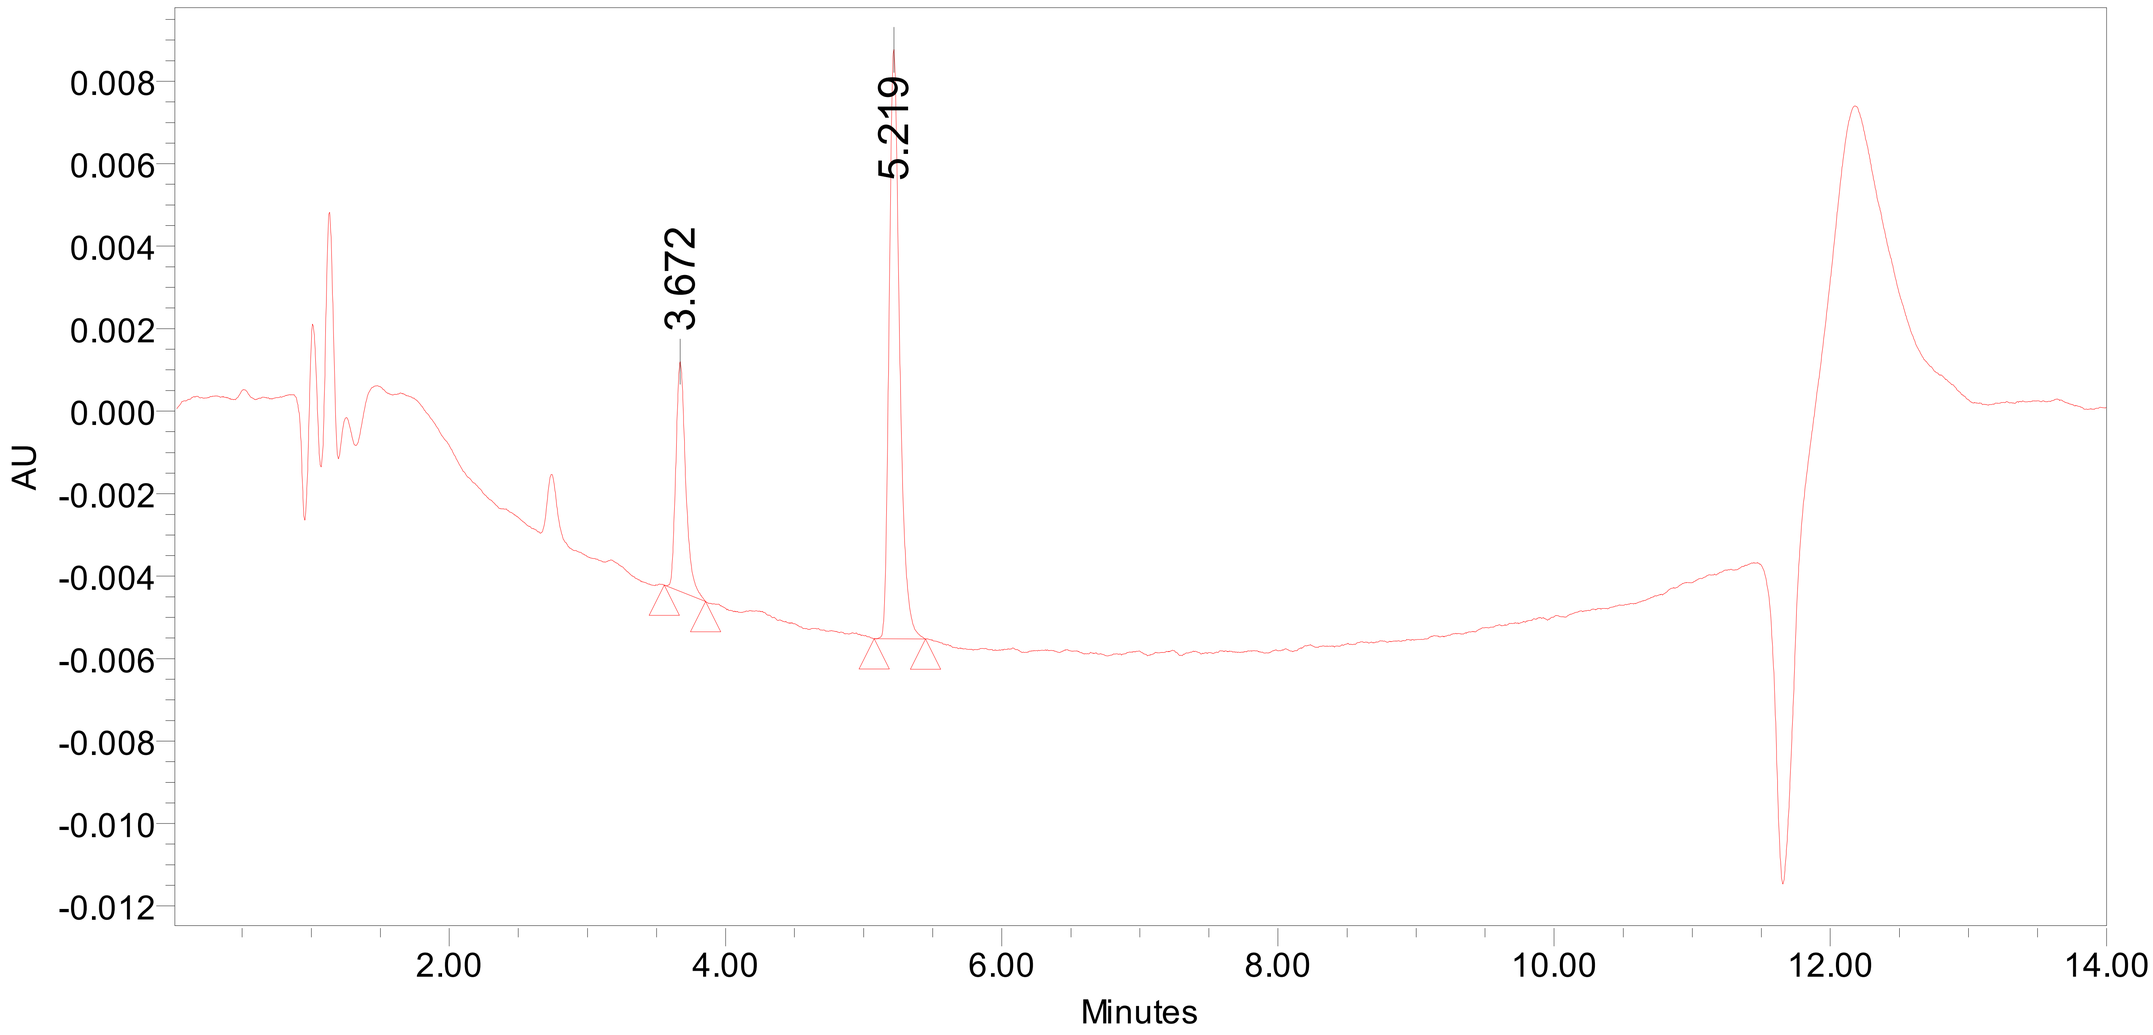

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.672	27639	5573		
2		5.219	75037	14288		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.672					
2		5.219					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_2 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-05 19:38:35 CET		
Date Processed:	2025-03-12 09:53:44 CET		

Auto-Scaled Chromatogram

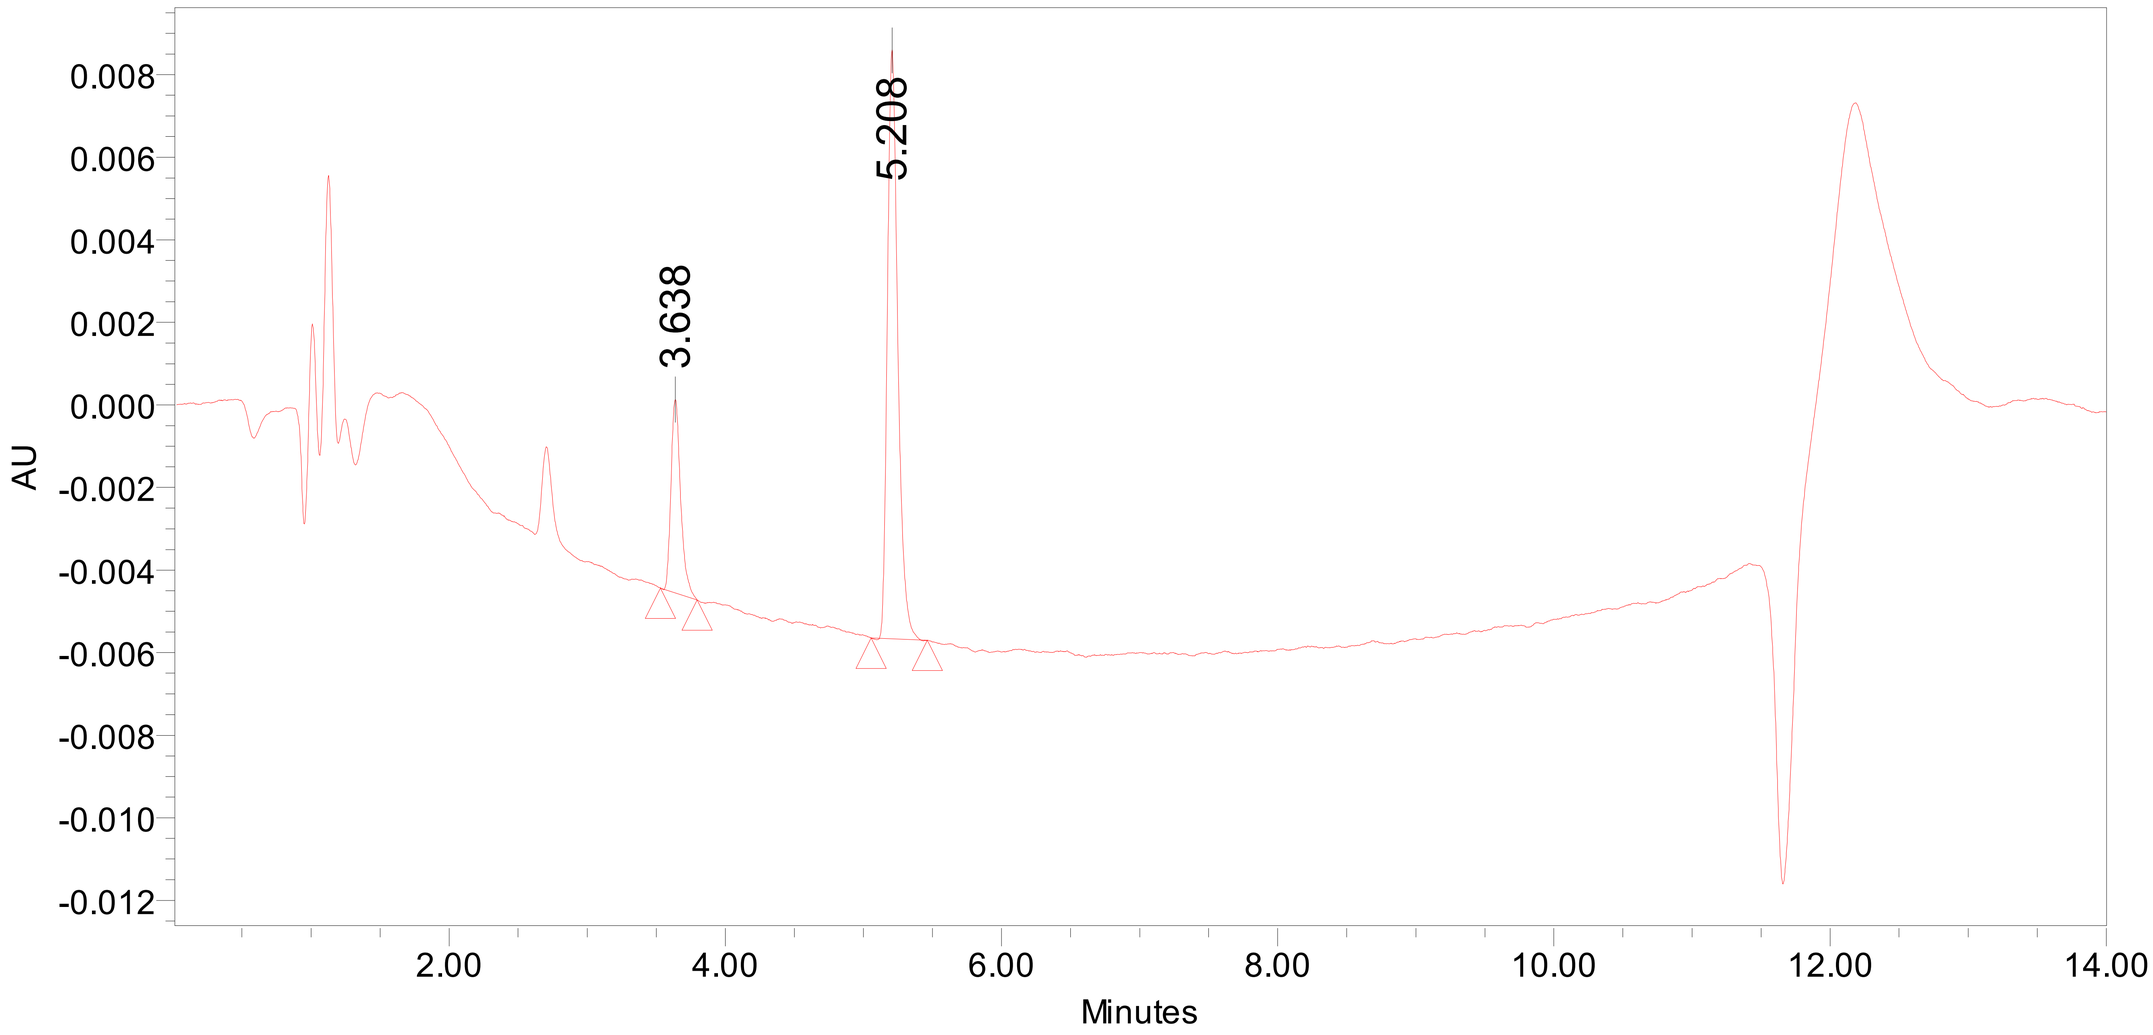

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.638	22879	4681		
2		5.208	74864	14277		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.638					
2		5.208					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_3 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-05 20:53:57 CET		
Date Processed:	2025-03-12 09:54:03 CET		

Auto-Scaled Chromatogram

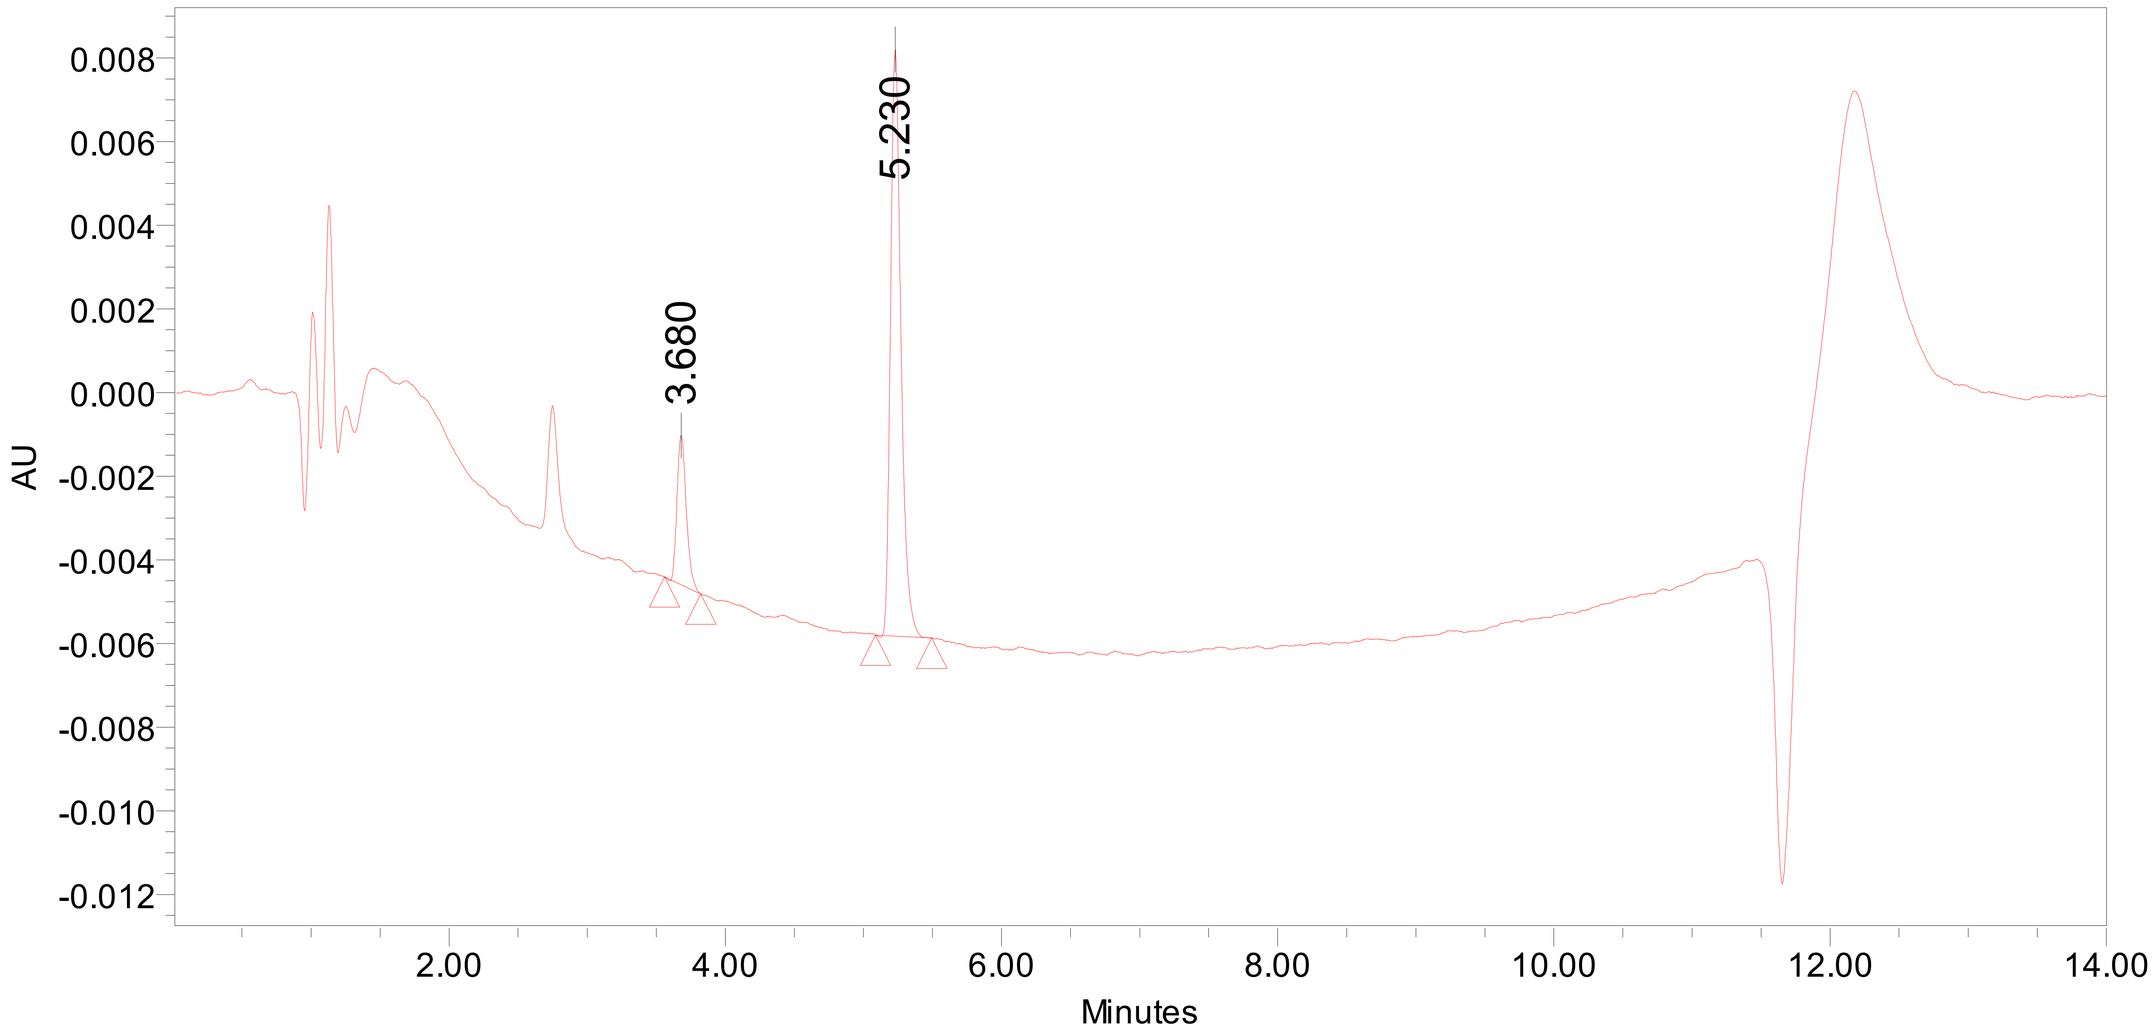

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.680	16710	3574		
2		5.230	73567	14023		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.680					
2		5.230					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_4 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-05 22:09:21 CET		
Date Processed:	2025-03-12 09:54:23 CET		

Auto-Scaled Chromatogram

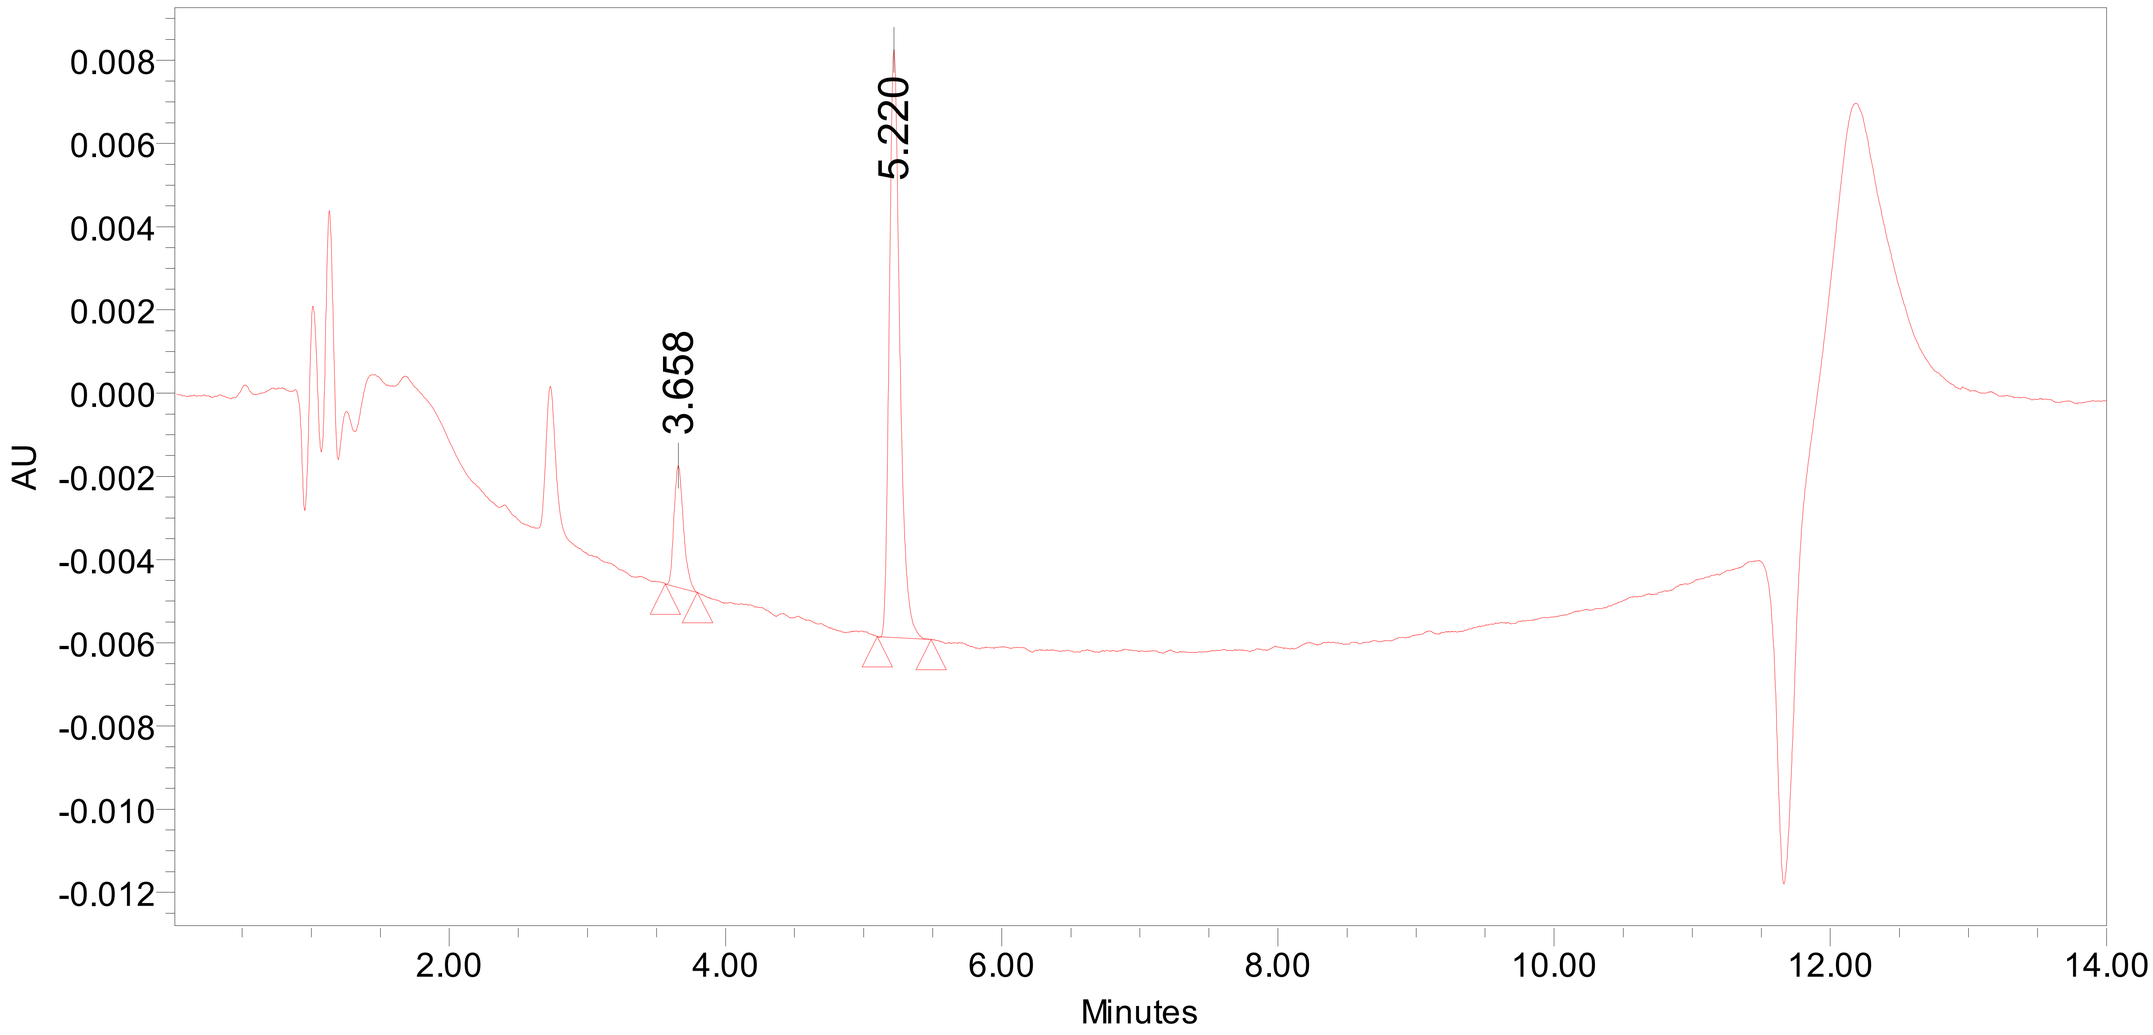

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.658	13989	2933		
2		5.220	74510	14133		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.658					
2		5.220					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_6 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-06 00:24:44 CET		
Date Processed:	2025-03-12 09:54:42 CET		

Auto-Scaled Chromatogram

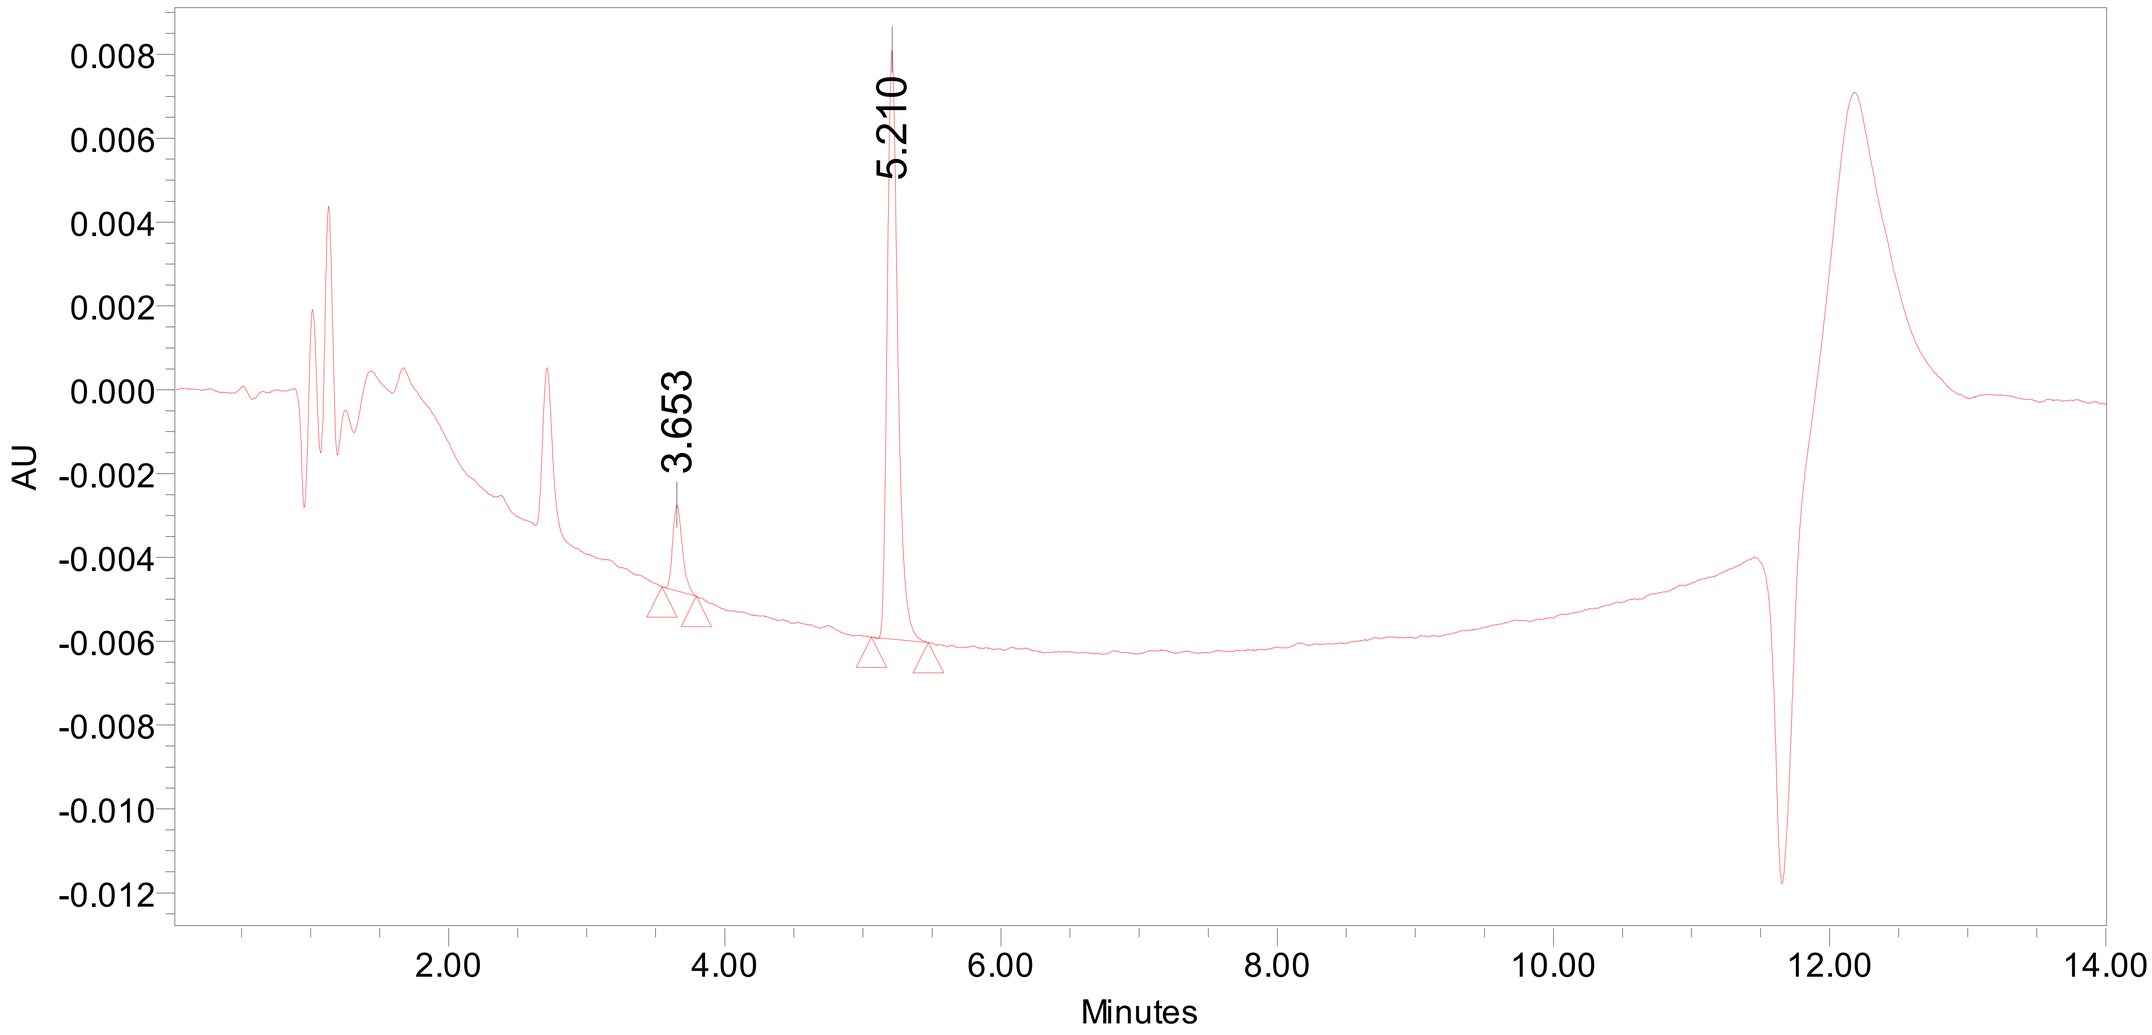

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.653	10016	2059		
2		5.210	74344	14063		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.653					
2		5.210					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_8 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-06 02:40:03 CET		
Date Processed:	2025-03-12 09:55:01 CET		

Auto-Scaled Chromatogram

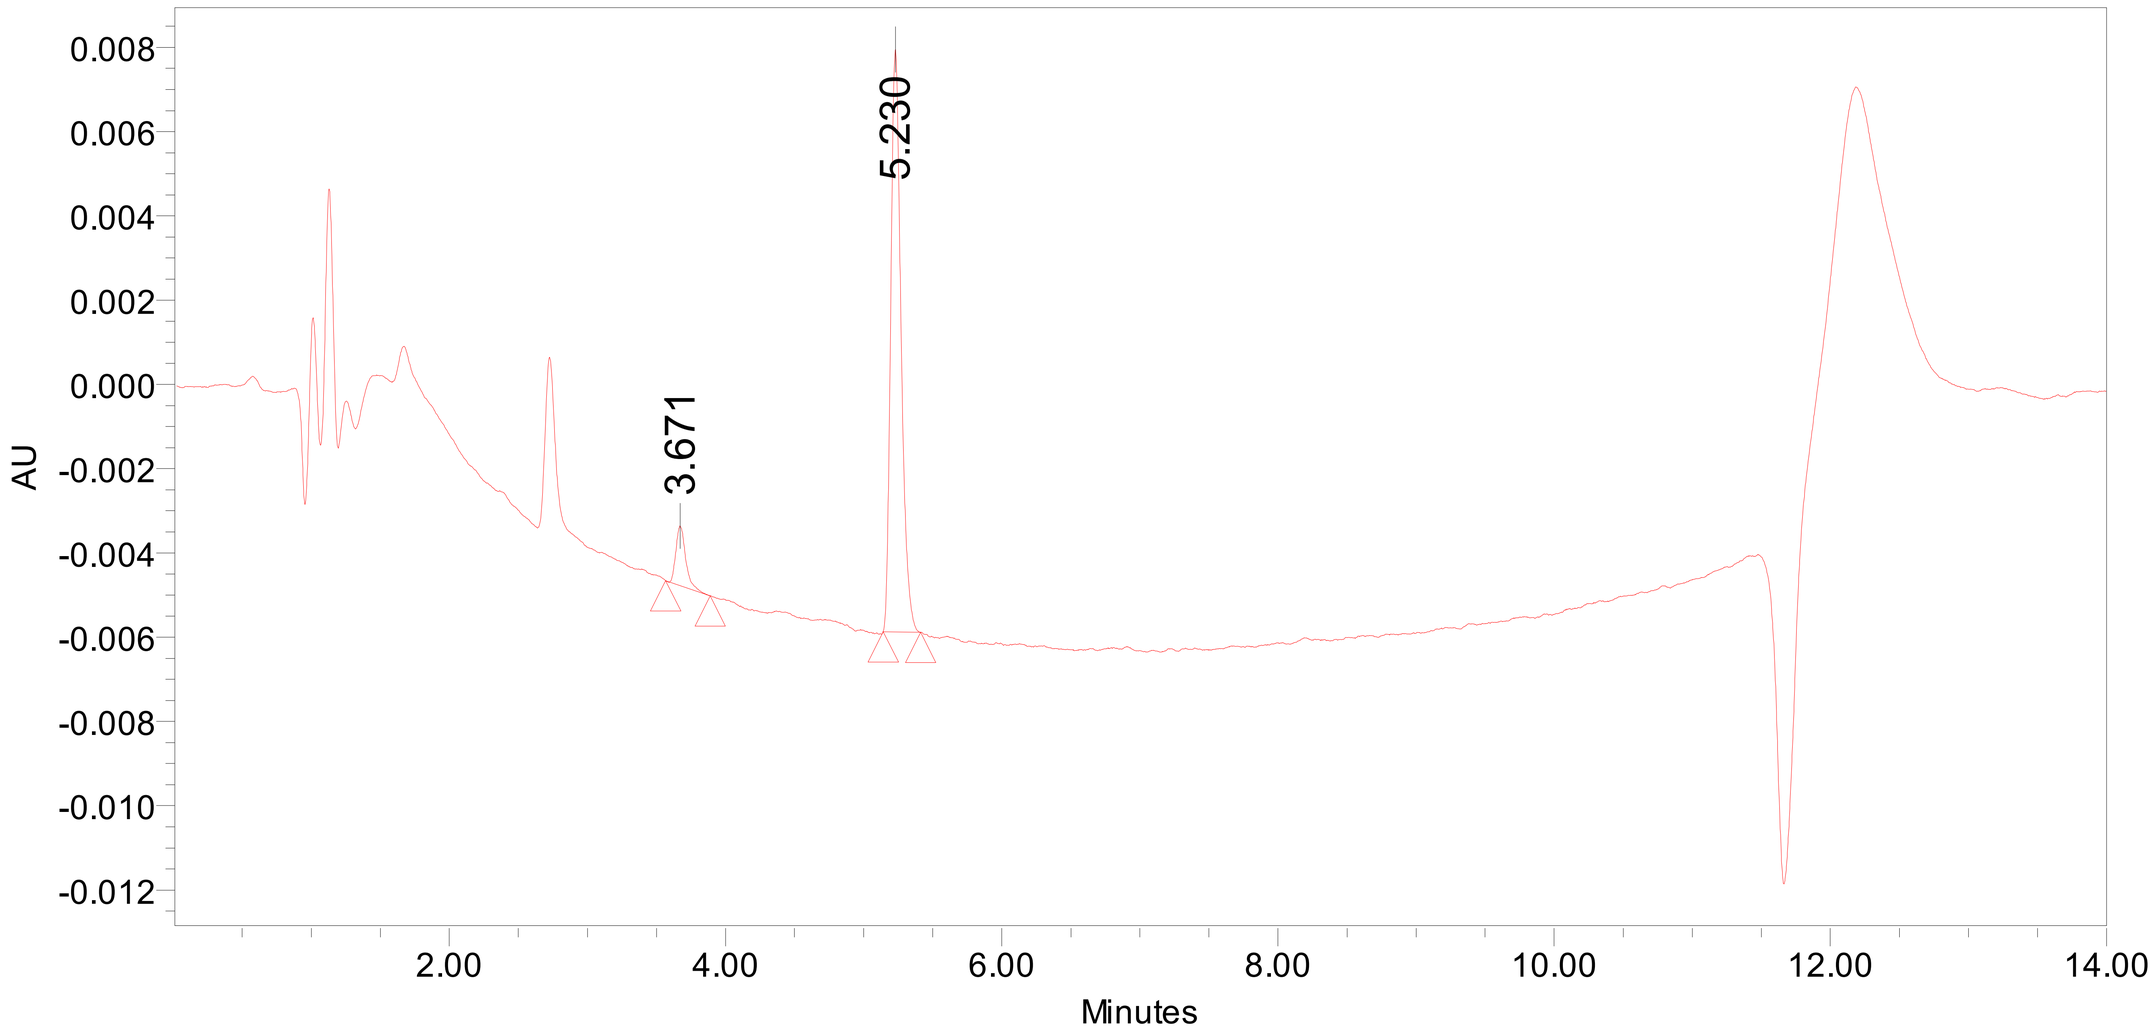

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.671	7028	1419		
2		5.230	71473	13822		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.671					
2		5.230					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_10 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-06 04:55:27 CET		
Date Processed:	2025-03-12 09:55:20 CET		

Auto-Scaled Chromatogram

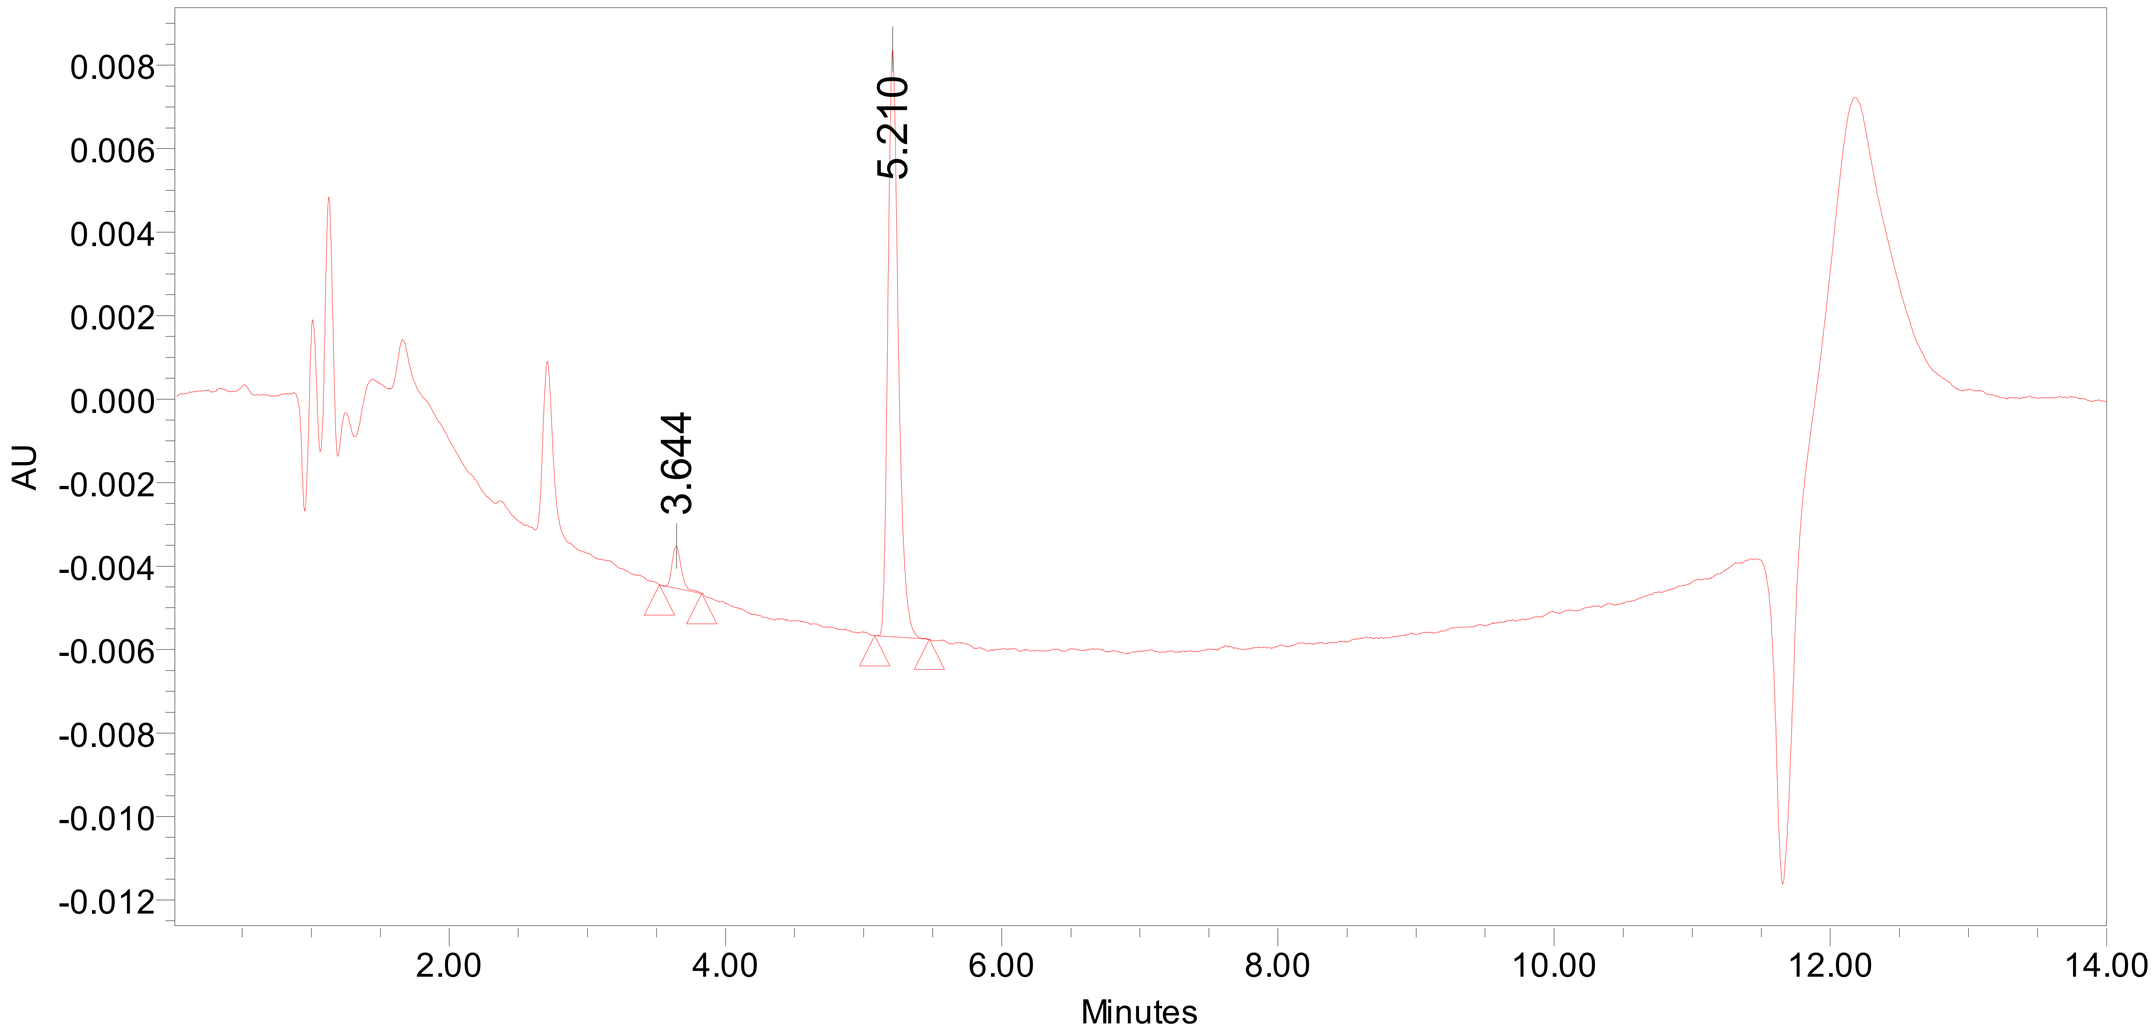

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.644	4638	1015		
2		5.210	73559	14068		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.644					
2		5.210					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_12 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-06 07:10:51 CET		
Date Processed:	2025-03-12 09:55:43 CET		

Auto-Scaled Chromatogram

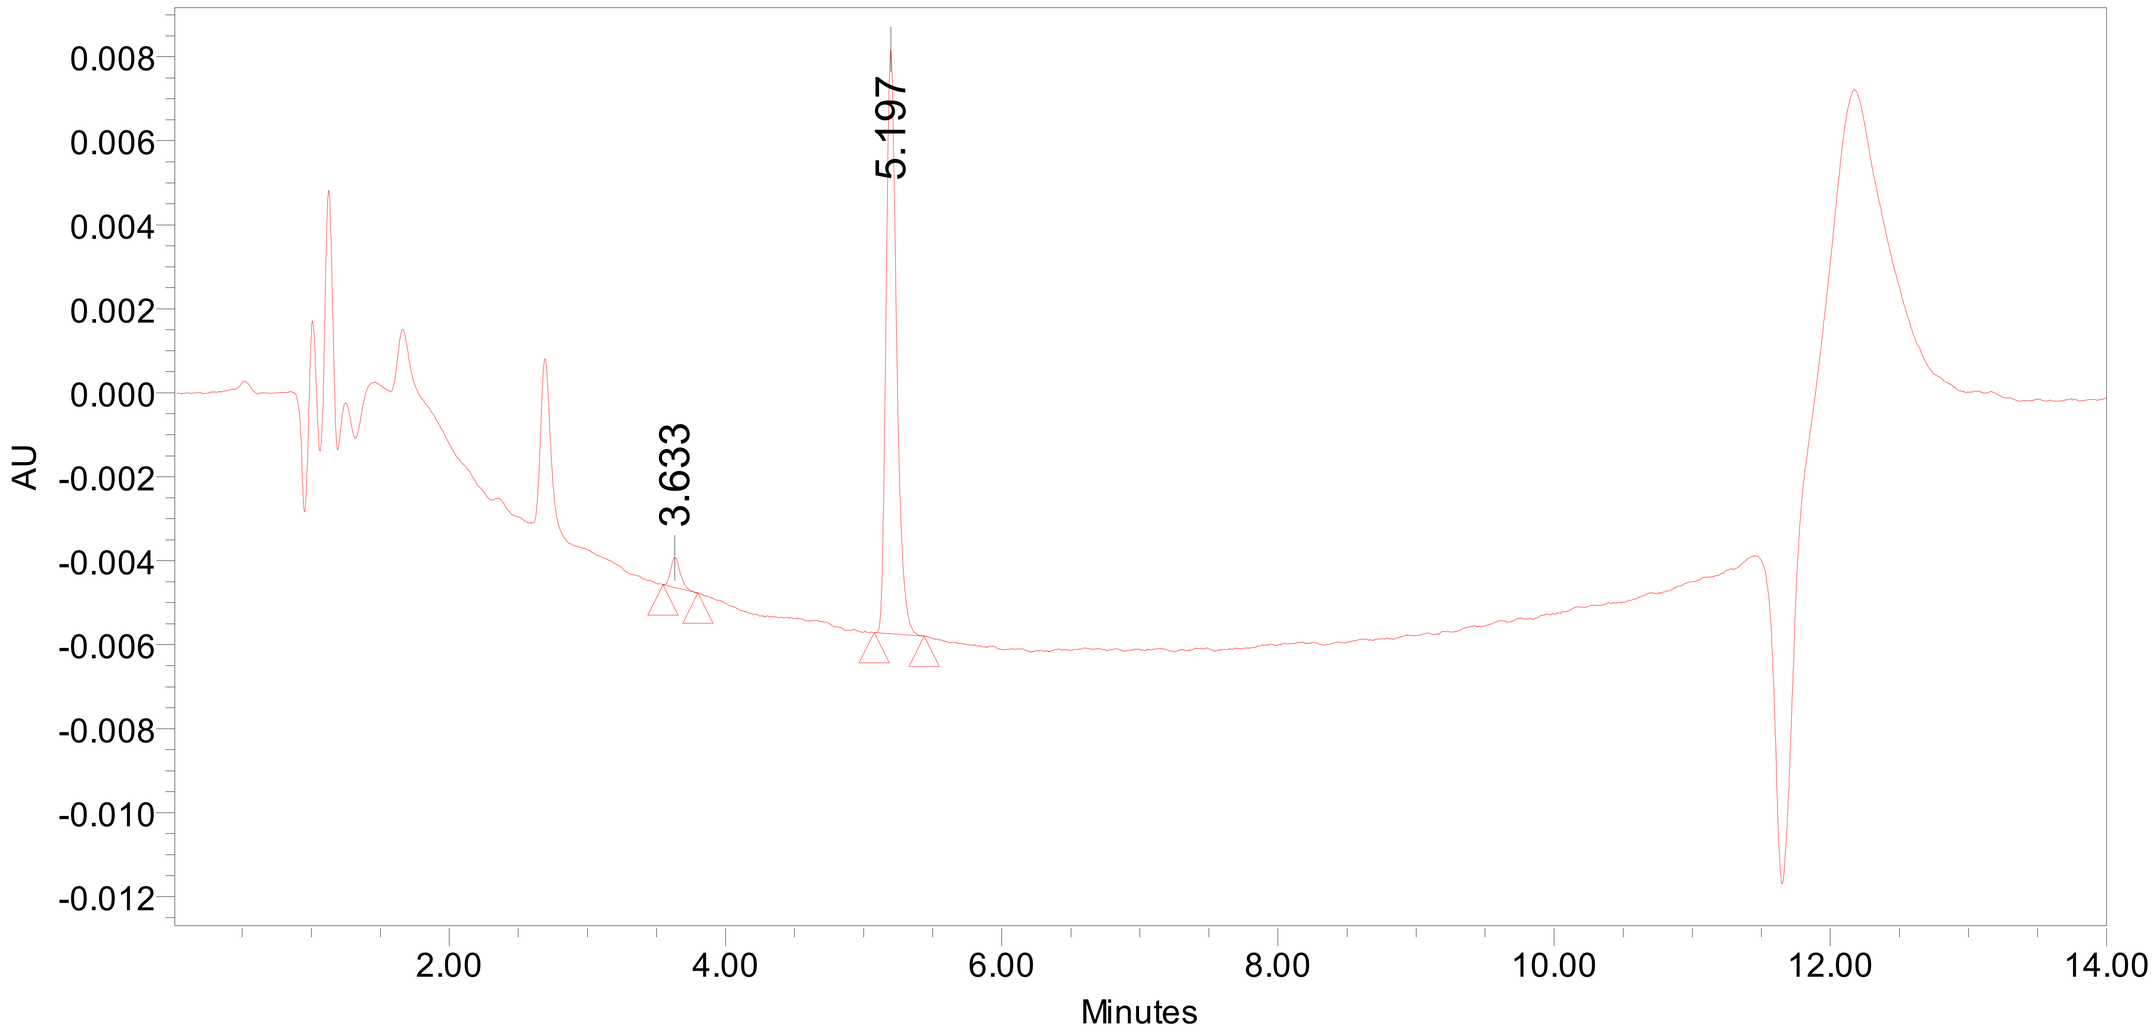

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.633	3449	706		
2		5.197	73084	13916		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.633					
2		5.197					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_16 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability hk21 every h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-06 11:26:12 CET		
Date Processed:	2025-03-12 09:56:02 CET		

Auto-Scaled Chromatogram

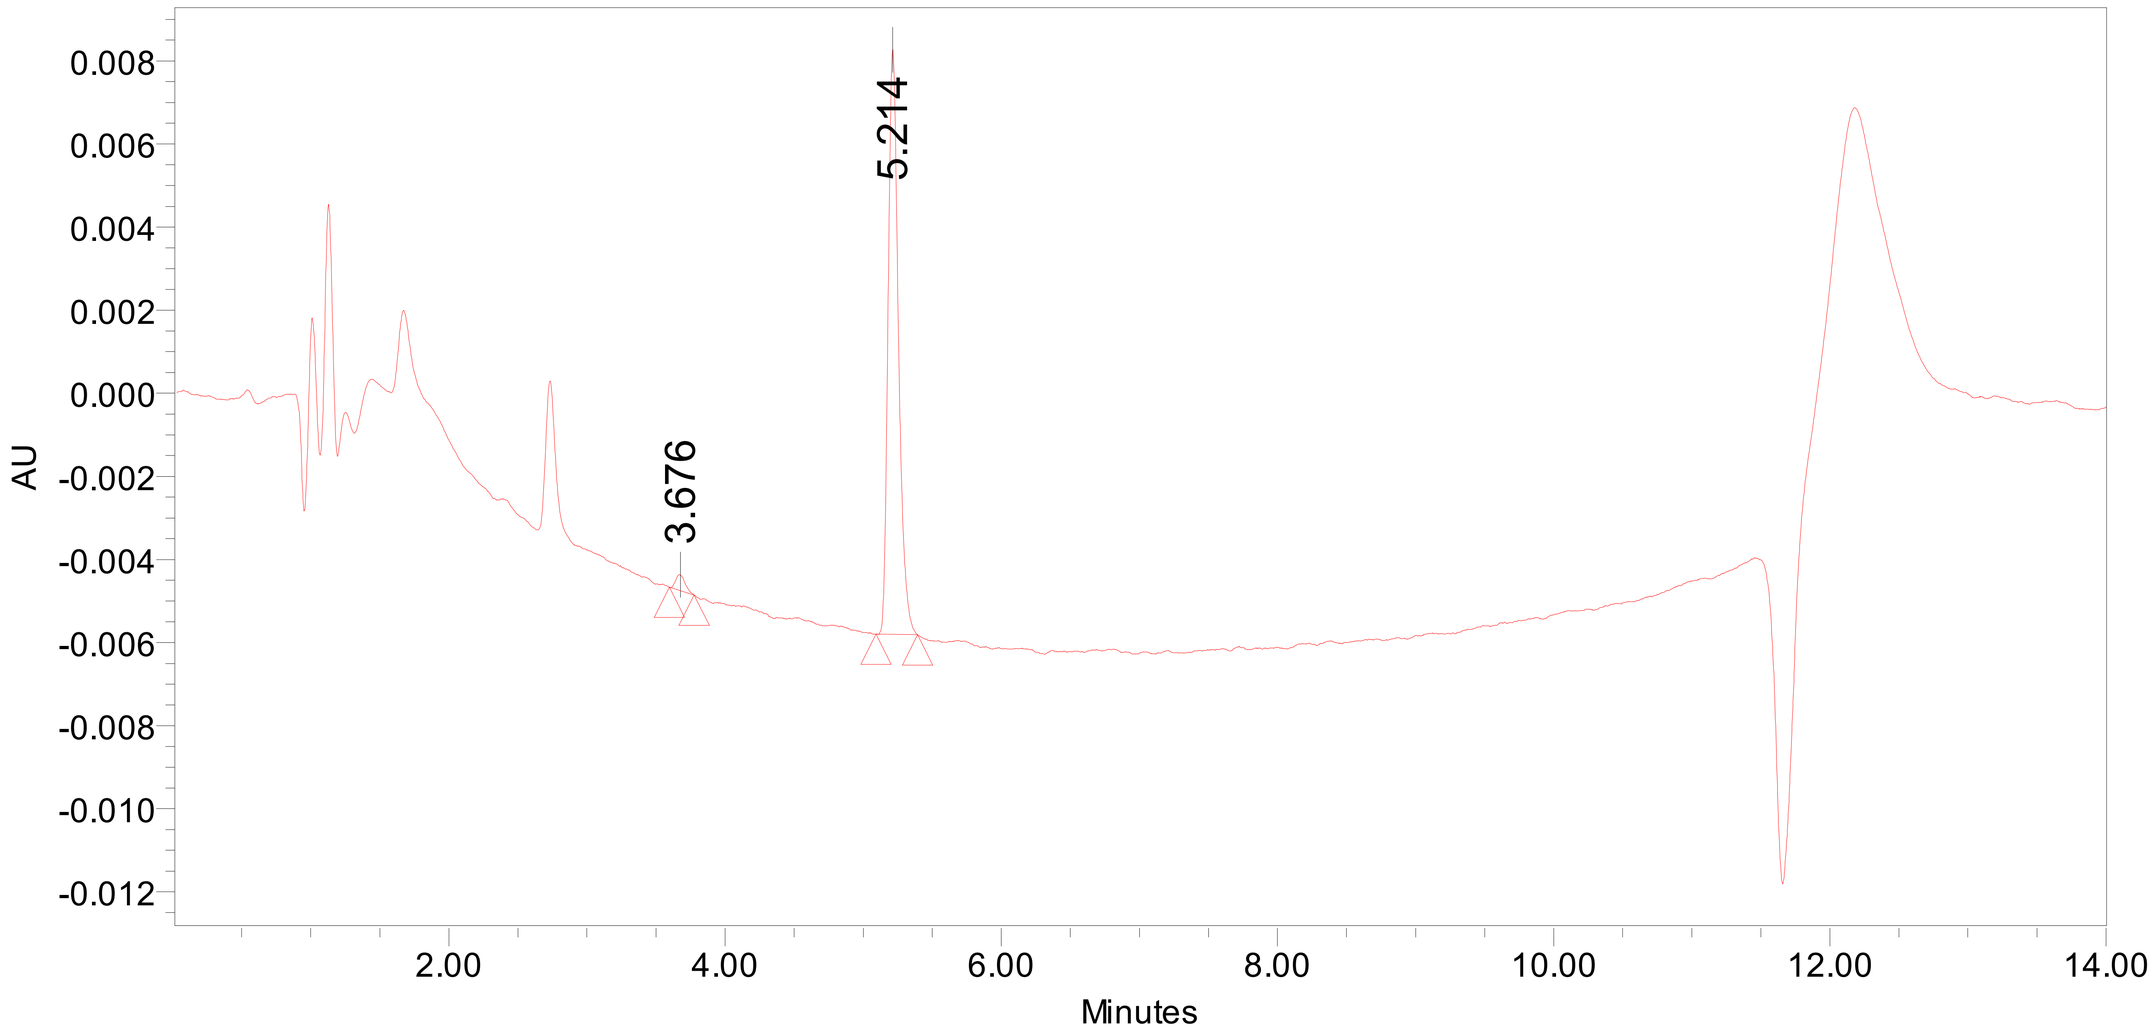

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.676	1792	382		
2		5.214	73176	14079		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.676					
2		5.214					

SAMPLE INFORMATION

Sample Name:	HK21_Stability again_24 h	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability again 24 h
Vial:	1	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	310.0nm
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 310.0 nm
Date Acquired:	2025-03-06 14:17:55 CET		
Date Processed:	2025-03-12 09:56:30 CET		

Auto-Scaled Chromatogram

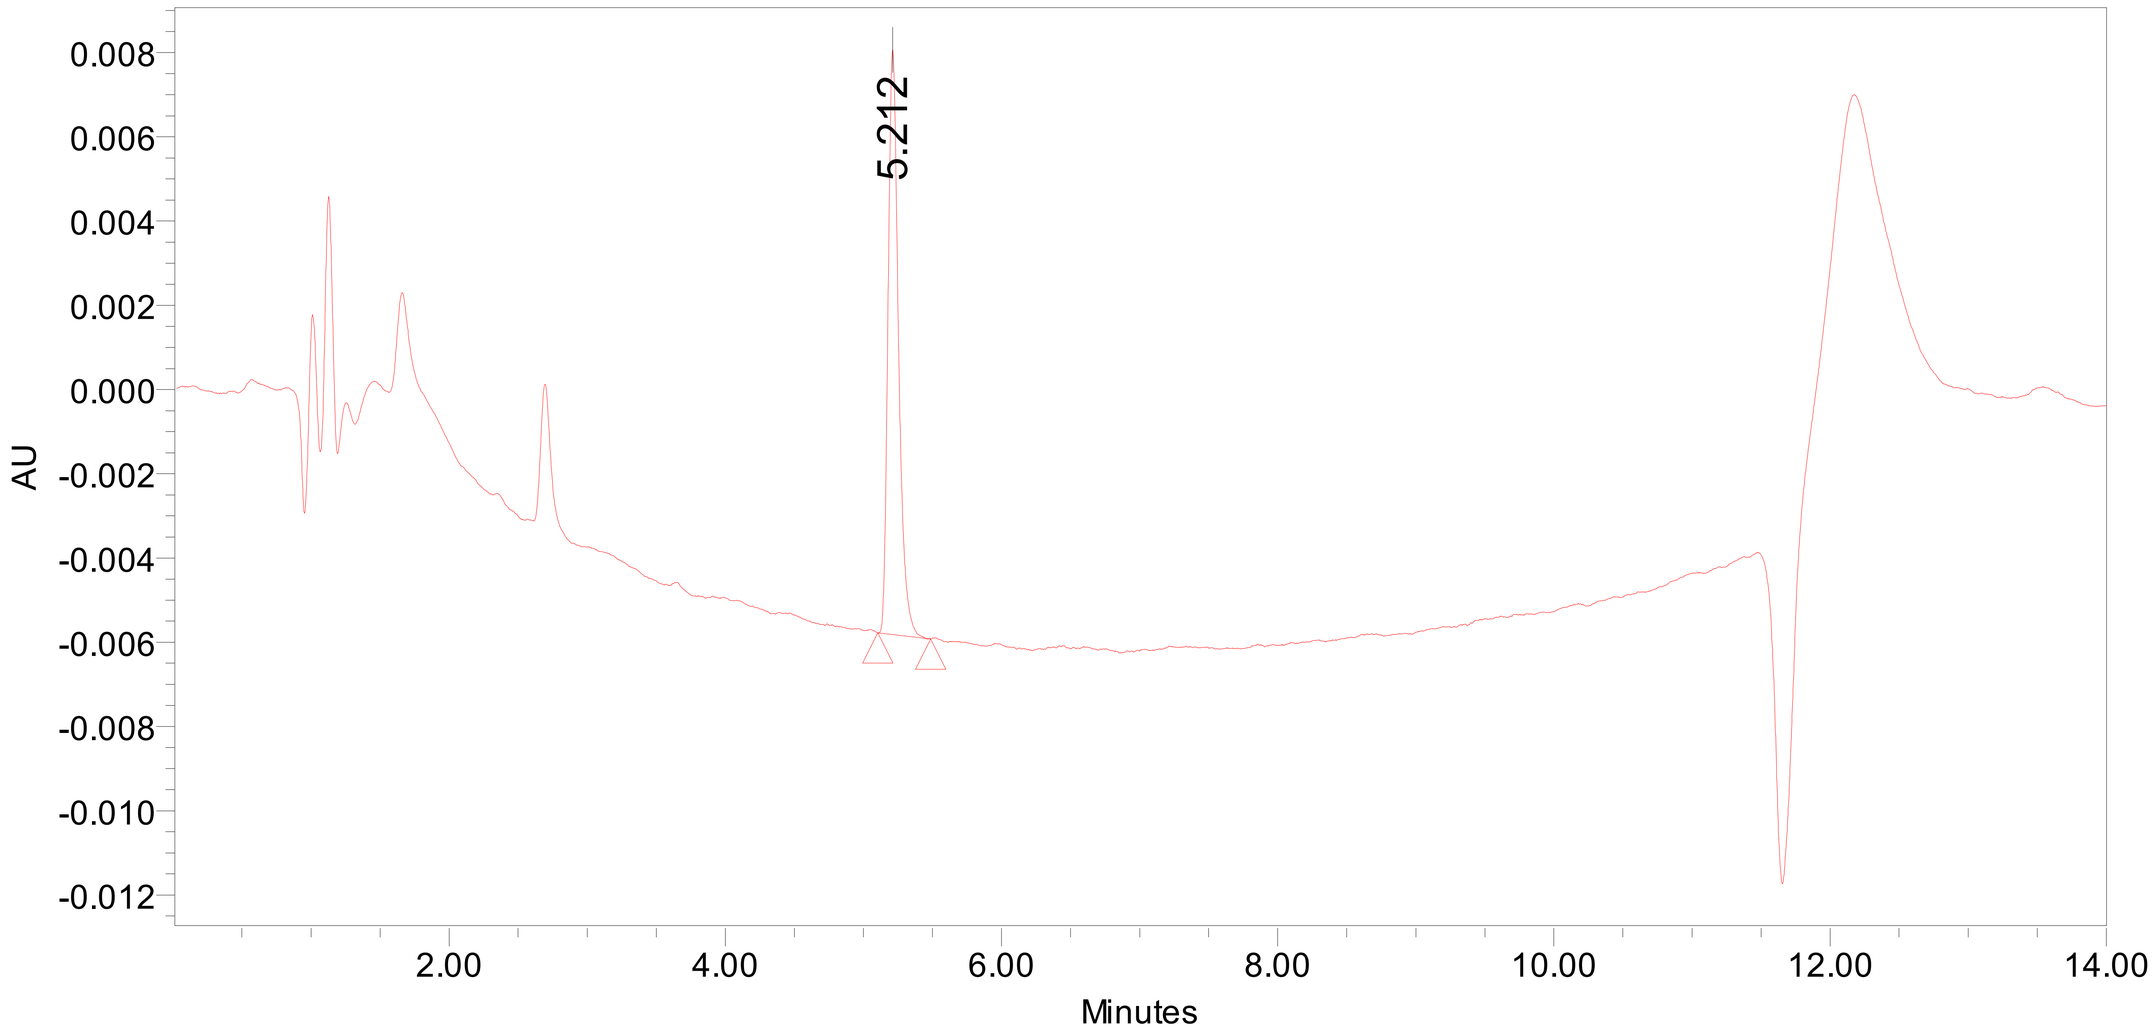

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.212	73125	13894		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.212					