
SAMPLE INFORMATION

Sample Name:	Hk14-Stability 2-time 0	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability repeat time 0
Vial:	105	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-15 13:37:54 CET		
Date Processed:	2025-01-20 14:39:40 CET		

Auto-Scaled Chromatogram

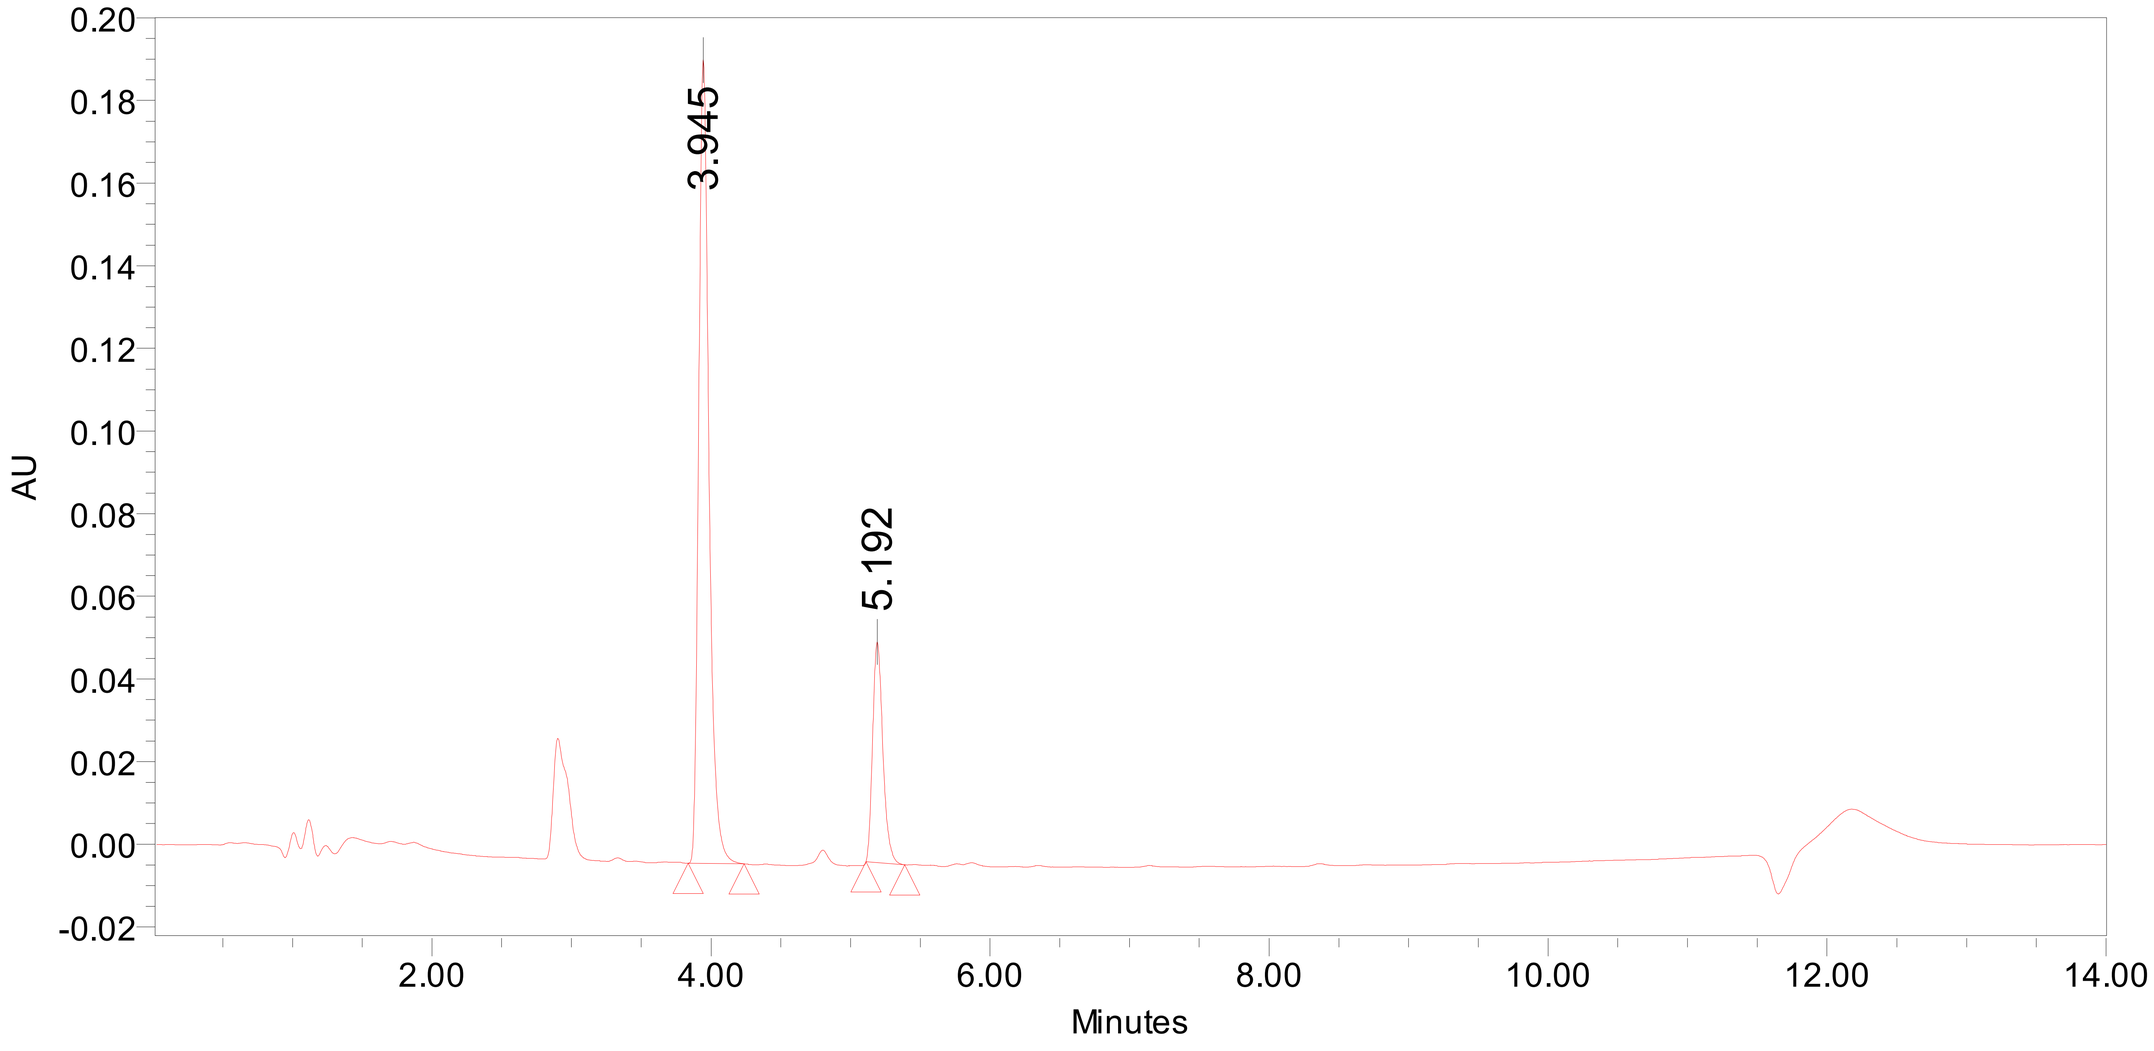

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.945	994742	194596		
2		5.192	271517	53426		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.945					
2		5.192					

SAMPLE INFORMATION

Sample Name:	HK14-Stability repeat-1 day	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	Stability repeat 1 day
Vial:	105	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-16 16:19:07 CET		
Date Processed:	2025-01-20 14:39:54 CET		

Auto-Scaled Chromatogram

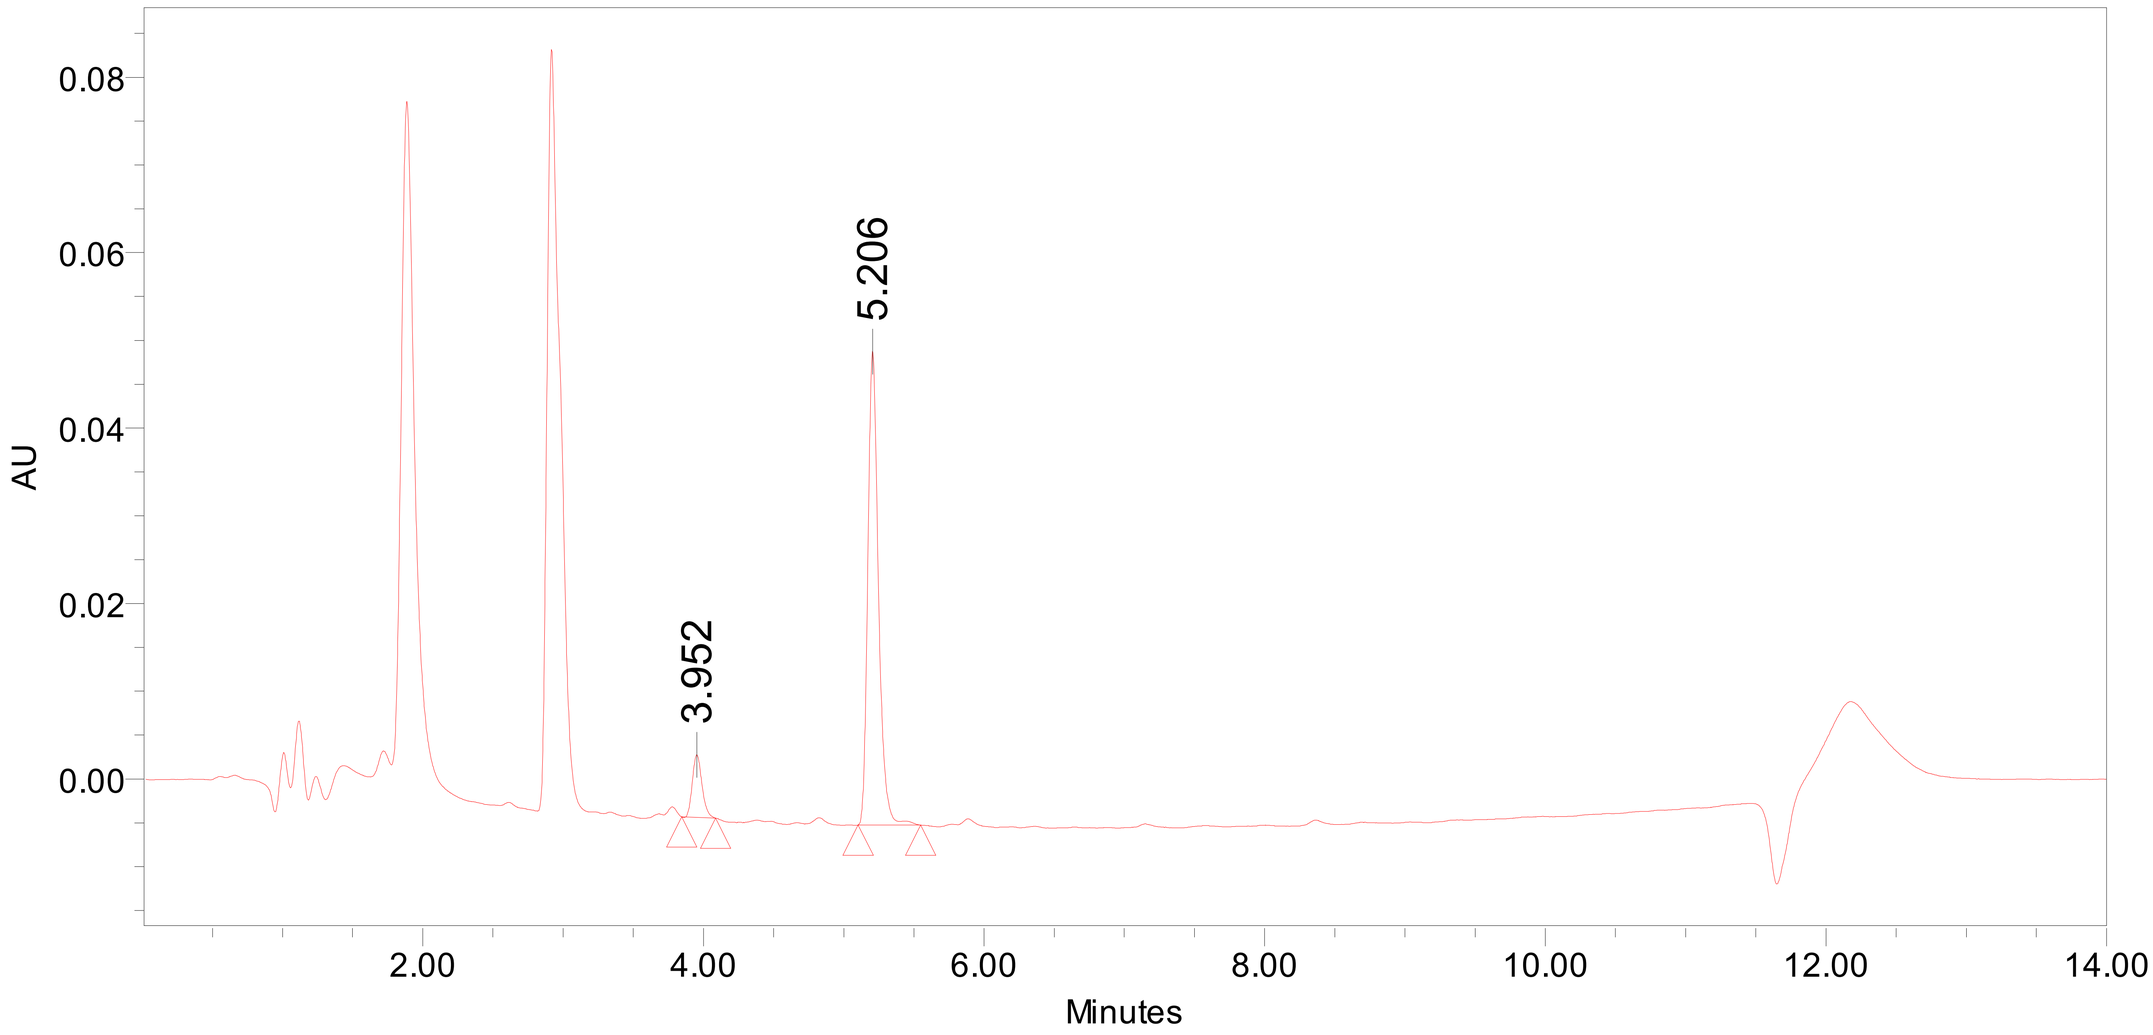

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.952	34323	7146		
2		5.206	286225	54005		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.952					
2		5.206					

SAMPLE INFORMATION

Sample Name:	HK14-Stability repeat-2 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability repeat 2 days
Vial:	105	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-17 18:15:43 CET		
Date Processed:	2025-01-20 14:40:26 CET		

Auto-Scaled Chromatogram

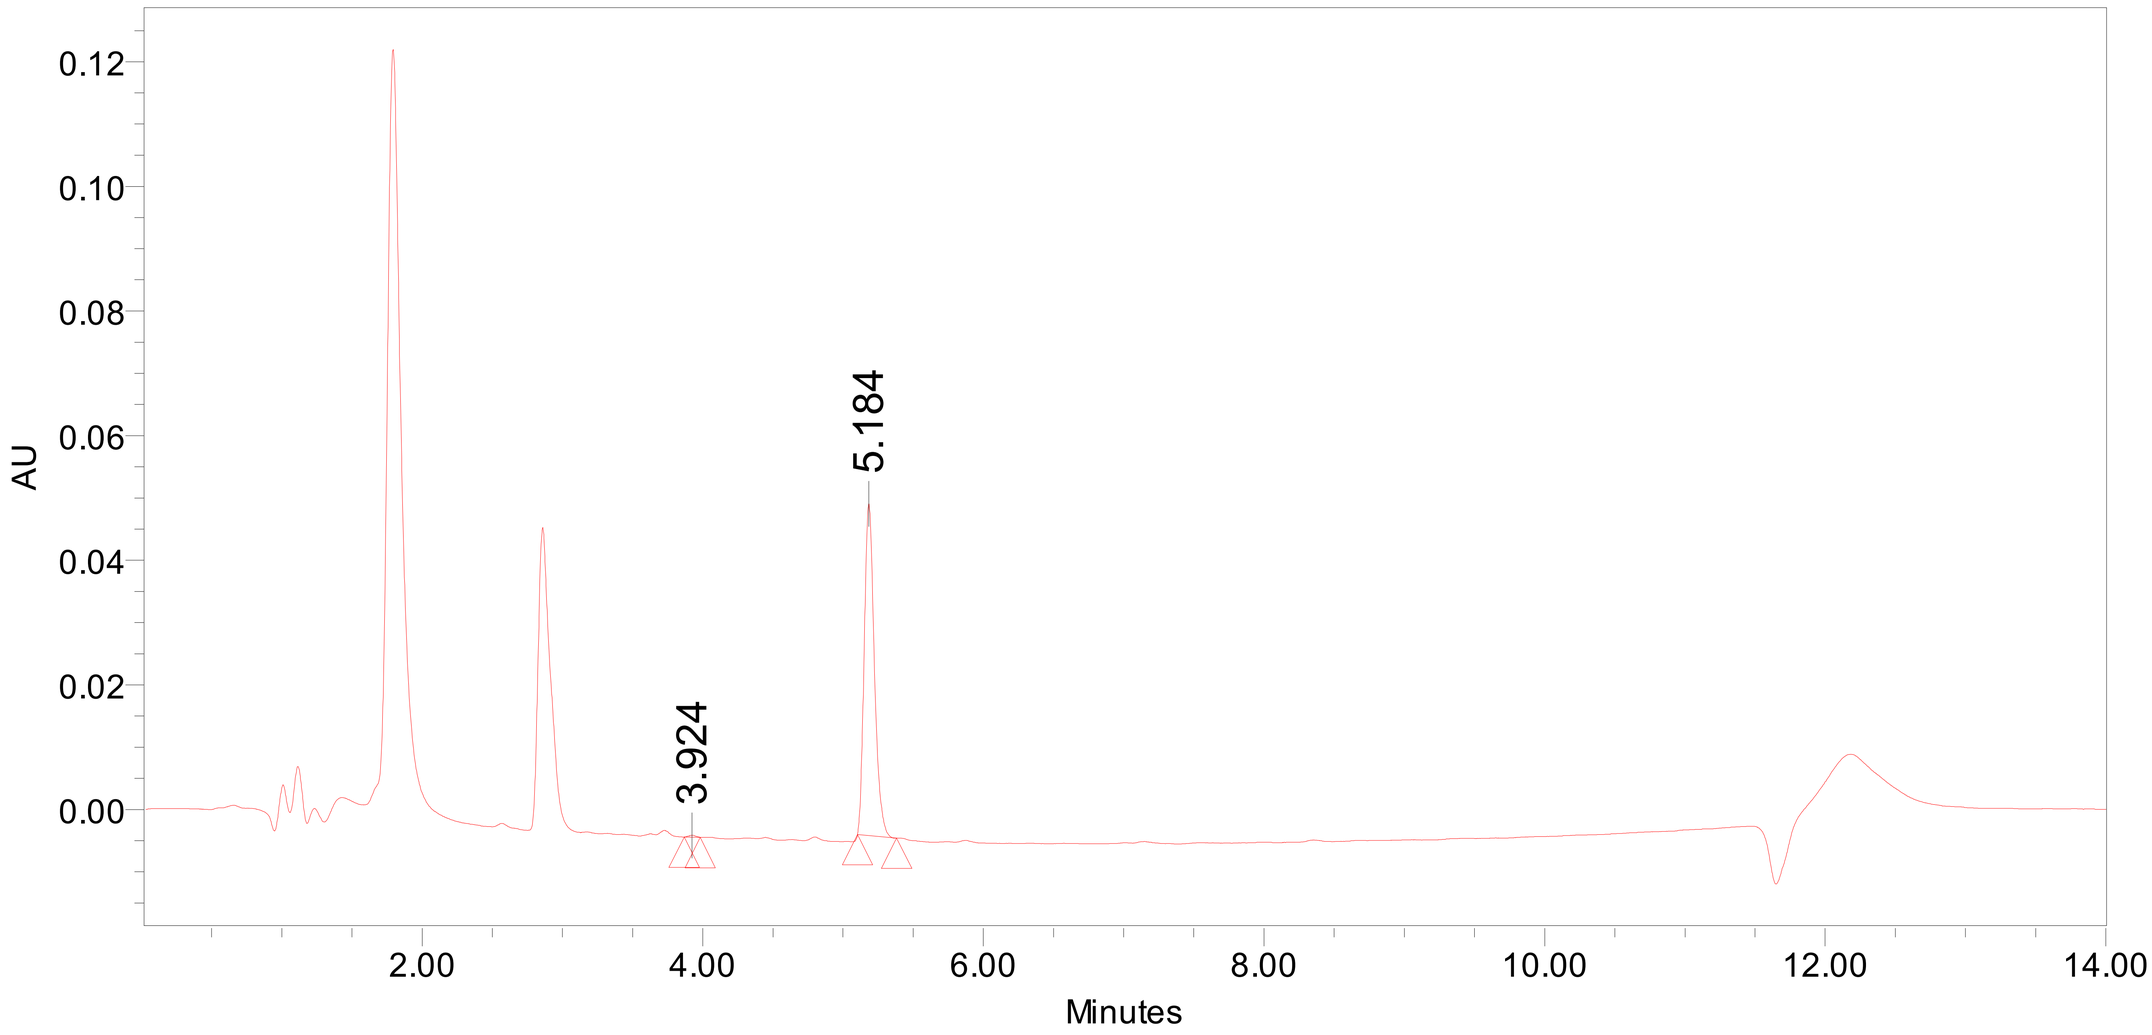

Peak Results

	Name	RT	Area	Height	Amount	Units
1		3.924	1113	307		
2		5.184	269733	53265		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		3.924					
2		5.184					

SAMPLE INFORMATION

Sample Name:	HK14-Stability repeat-3 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability repeat 3 days
Vial:	105	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-18 18:24:05 CET		
Date Processed:	2025-01-20 14:41:54 CET		

Auto-Scaled Chromatogram

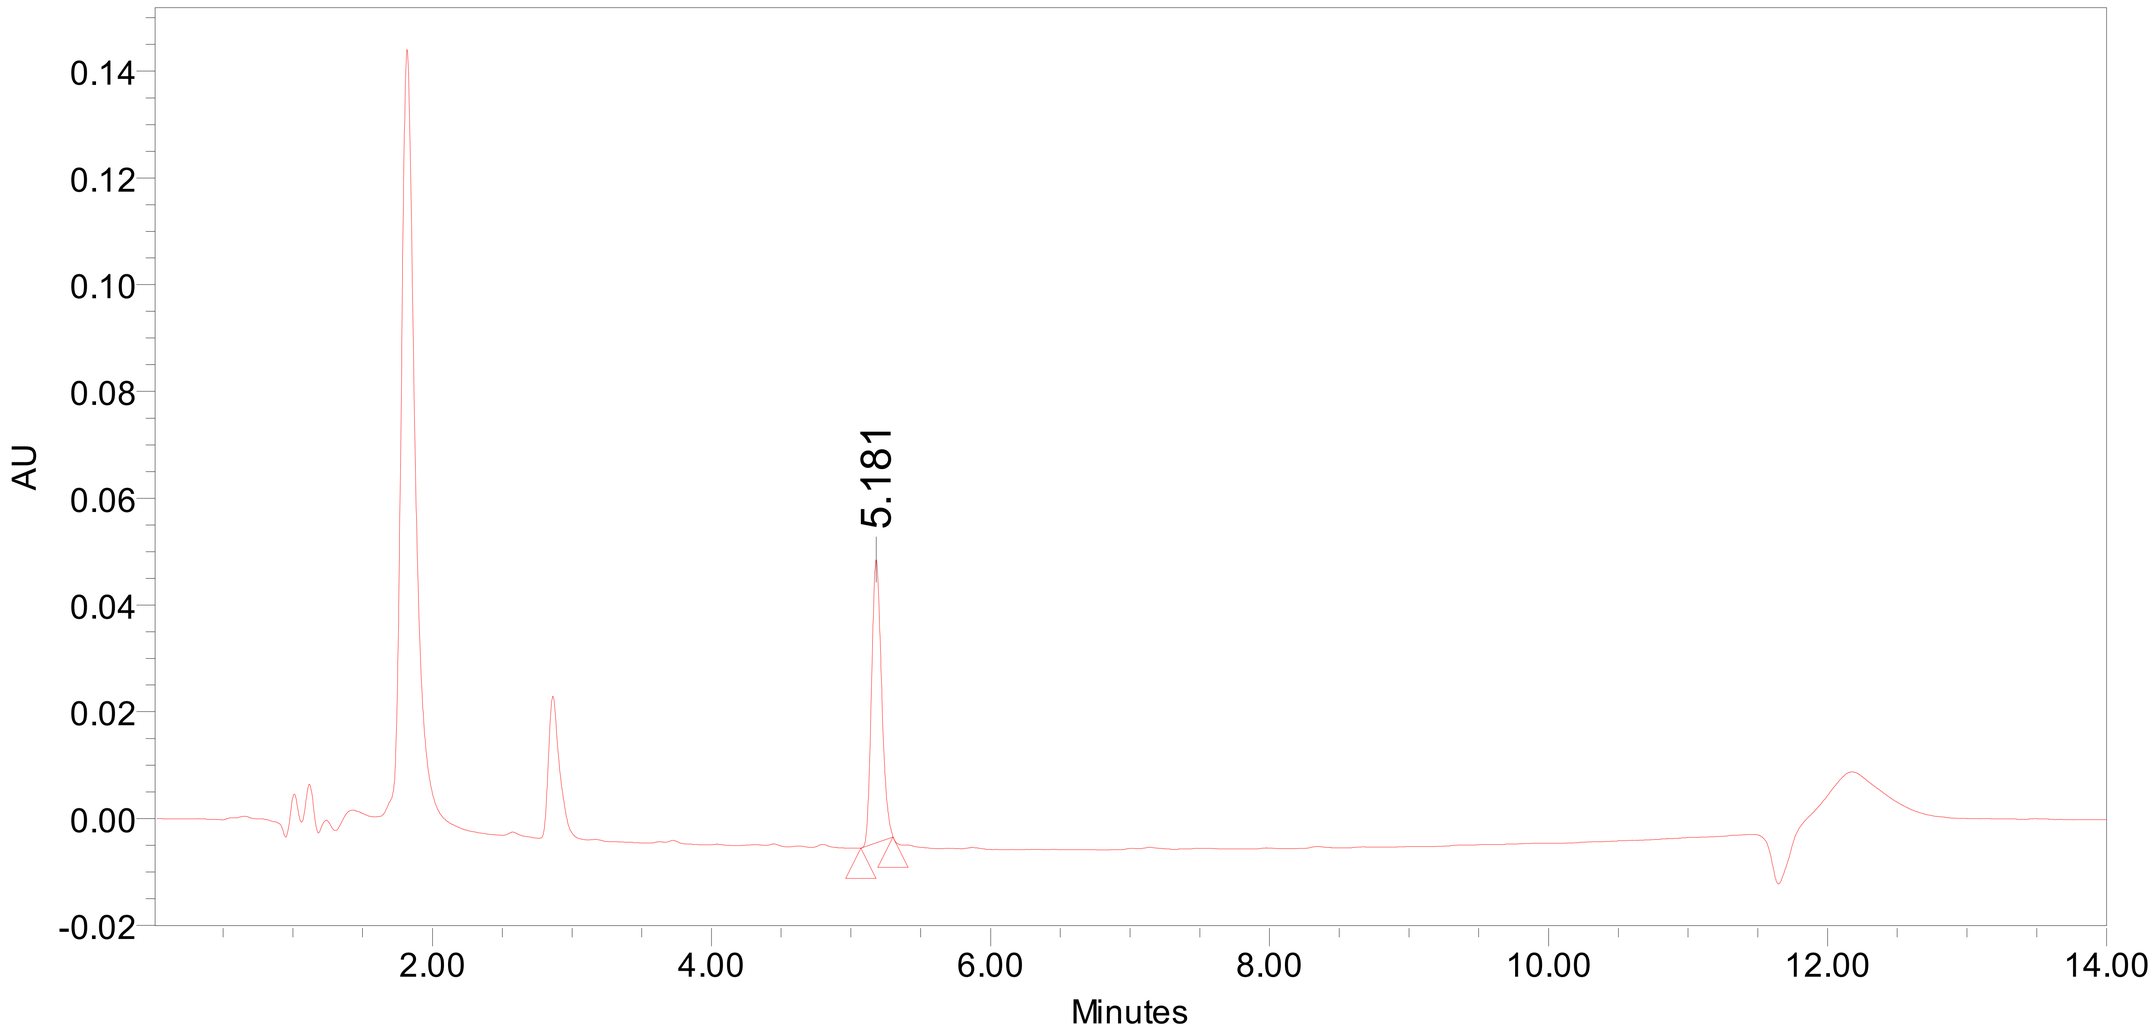

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.181	265742	53061		


PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.181					

SAMPLE INFORMATION

Sample Name:	HK14-Stability repeat-4 days	Acquired By:	System
Sample Type:	Unknown	Sample Set Name:	stability 4 days
Vial:	105	Acq. Method Set:	AB_95 in 10_total 12
Injection #:	1	Processing Method:	Anna General PM
Injection Volume:	15.00 ul	Channel Name:	280.0nm@1
Run Time:	14.0 Minutes	Proc. Chnl. Descr.:	PDA 280.0 nm
Date Acquired:	2025-01-19 17:45:15 CET		
Date Processed:	2025-01-20 14:42:08 CET		

Auto-Scaled Chromatogram

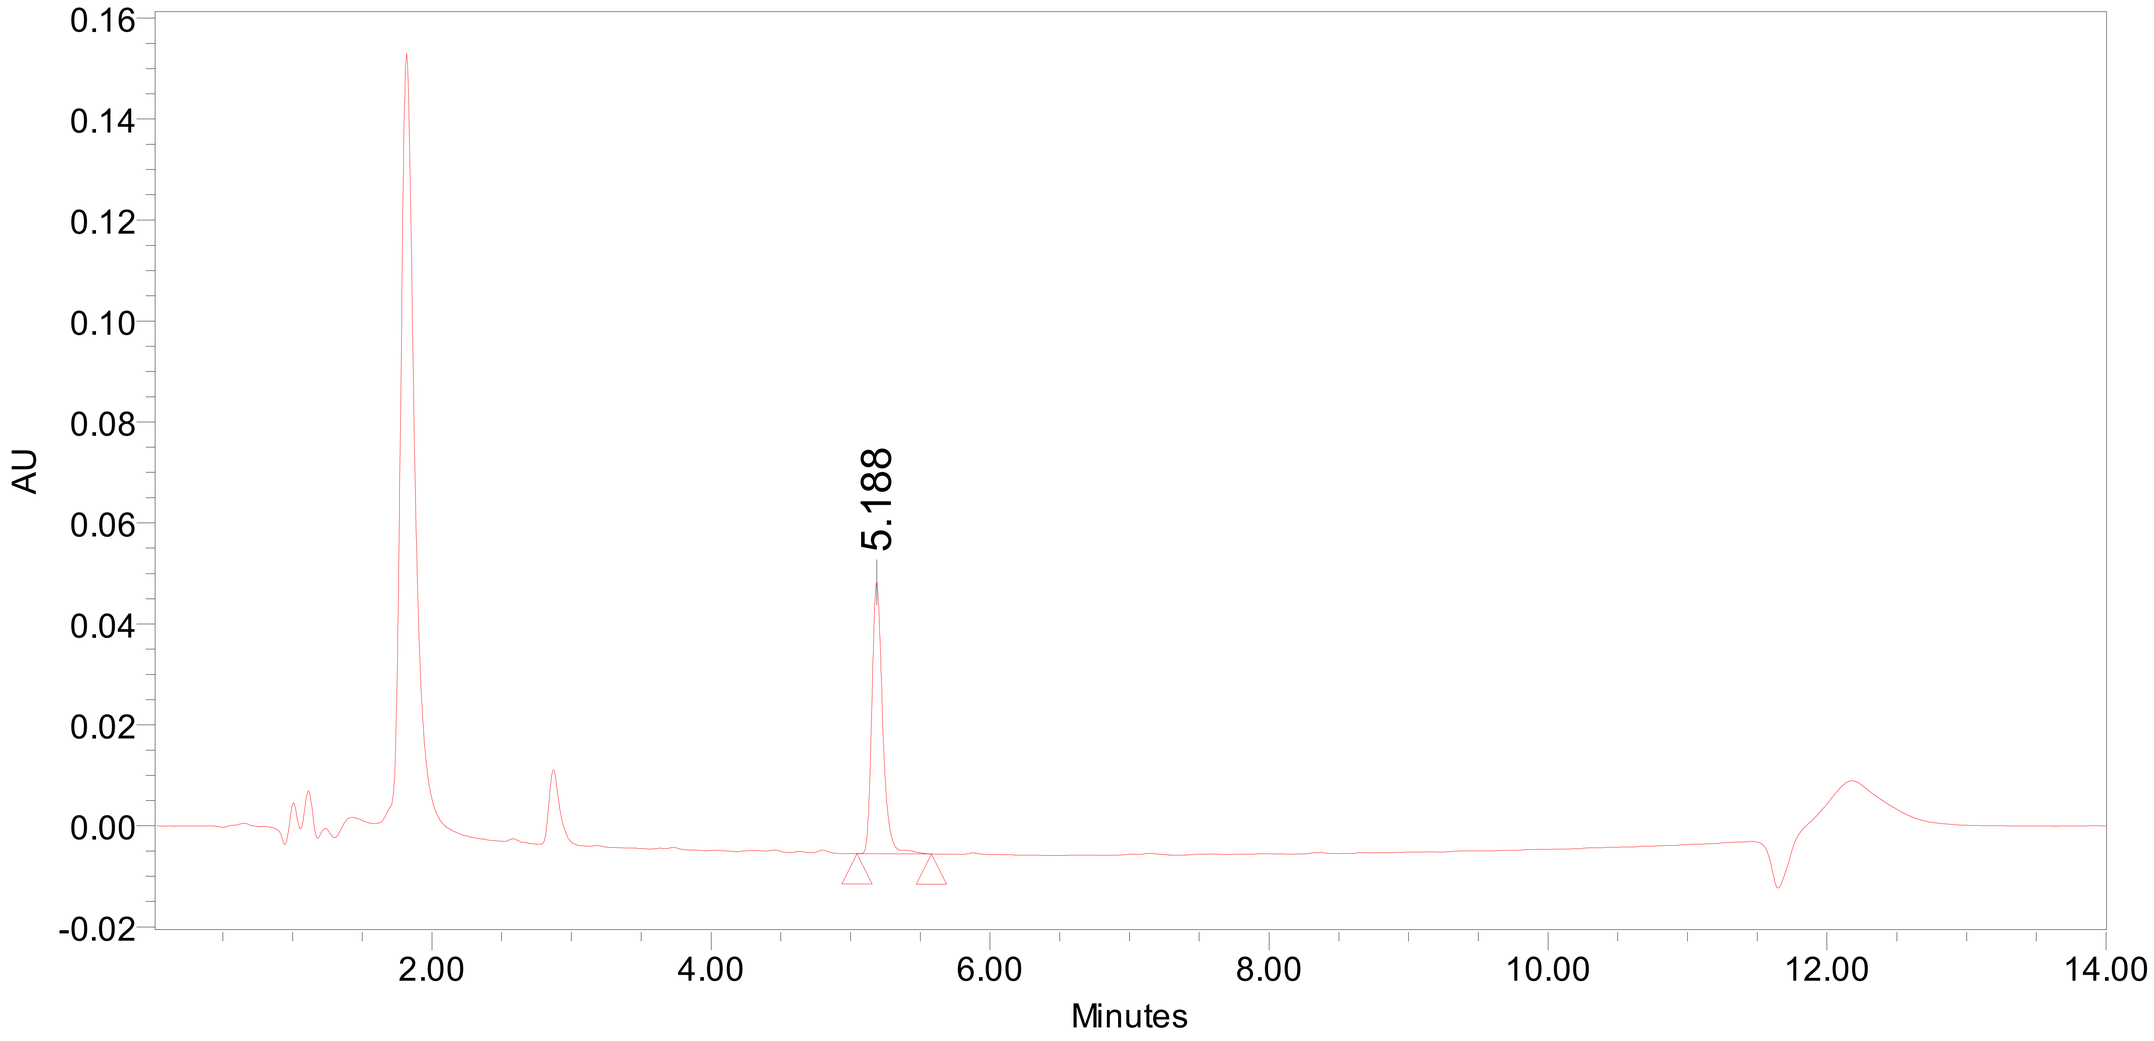

Peak Results

	Name	RT	Area	Height	Amount	Units
1		5.188	288068	53802		

PDA Result Table

	Name	RT	Purity1 Angle	Purity1 Threshold	Match1 Spect. Name	Match1 Angle	Match1 Threshold
1		5.188					